

Agilent 1100 Series Isocratic Pump



Reference Manual



Agilent Technologies

Notices

© Agilent Technologies, Inc. 2002

No part of this manual may be reproduced in any form or by any means (including electronic storage and retrieval or translation into a foreign language) without prior agreement and written consent from Agilent Technologies, Inc. as governed by United States and international copyright laws.

Manual Part Number

G1310-90003

Edition

Edition 07/02

Printed in Germany

Agilent Technologies
Hewlett-Packard-Strasse 8
76337 Waldbronn, Germany

Software Revision

This guide is valid for A.01.xx revisions of the Agilent 1100 Series Isocratic Pump software, where xx refers to minor revisions of the software that do not affect the technical accuracy of this guide.

Warranty

The material contained in this document is provided “as is,” and is subject to being changed, without notice, in future editions. Further, to the maximum extent permitted by applicable law, Agilent disclaims all warranties, either express or implied, with regard to this manual and any information contained herein, including but not limited to the implied warranties of merchantability and fitness for a particular purpose. Agilent shall not be liable for errors or for incidental or consequential damages in connection with the furnishing, use, or performance of this document or of any information contained herein. Should Agilent and the user have a separate written agreement with warranty terms covering the material in this document that conflict with these terms, the warranty terms in the separate agreement shall control.

Technology Licenses

The hardware and/or software described in this document are furnished under a license and may be used or copied only in accordance with the terms of such license.

Restricted Rights Legend

Software and technical data rights granted to federal government customers include only those rights customarily provided to end user Customers of Software. Agilent provides this customary commercial license in Software and technical data pursuant to FAR 12.211 (Technical Data) and FAR 12.212 (Computer Software) and, for Department of Defense purchases, DFARS 252.227-7015 (Technical Data - Commercial Items) and DFARS 227.7202-3 (Rights in Commercial Computer Software or Computer Software Documentation). If a federal government or other public sector Customer has a need for

rights not conveyed under these terms, it must negotiate with Agilent to establish acceptable terms in a written agreement executed by all relevant parties.

Safety Notices

CAUTION

A **CAUTION** notice denotes a hazard. It calls attention to an operating procedure, practice, or the like that, if not correctly performed or adhered to, could result in damage to the product or loss of important data. Do not proceed beyond a **CAUTION** notice until the indicated conditions are fully understood and met.

WARNING

A **WARNING** notice denotes a hazard. It calls attention to an operating procedure, practice, or the like that, if not correctly performed or adhered to, could result in personal injury or death. Do not proceed beyond a **WARNING** notice until the indicated conditions are fully understood and met.

In This Guide...

1 Installing the Pump

How to install the isocratic pump

2 Optimizing Performance

How to optimize the isocratic pump to achieve best chromatographic results

3 Troubleshooting and Test Functions

The isocratic pump's built-in troubleshooting and test functions

4 Repairing the Pump

Instructions on simple, routine repair procedures as well as more extensive repairs requiring exchange of internal parts

5 Parts and Materials

Detailed illustrations and lists for identification of parts and materials

6 Introduction to the Isocratic Pump

An introduction to the pump, instrument overview, theory of operation, external communication and internal connectors

7 Control Module Screens for the Isocratic Pump

This chapter is intended to introduce an operator to the screens available for operation of the Agilent 1100 isocratic pump with the Agilent 1100 control module.

Please use the manual of the control module for further detailed reference.

8 Specifications

Performance specifications of the isocratic pump

Contents

1 Installing the Pump

- Site Requirements 12
- Unpacking the Isocratic Pump 15
- Optimizing the Stack Configuration 17
- Installing the Isocratic Pump 19
- Flow Connections of the Isocratic Pump 22
- Priming and Purging the System 25

2 Optimizing Performance

- Hints for Successful Use of the Isocratic Pump 30
- Solvent Information 31
- Prevent Blocking of Solvent Filters 32
- When to Use a Vacuum Degasser 34
- When to use the Continuous Seal Wash Option 35
- When to Use Alternative Seals 36
- How to Optimize the Compressibility Compensation Setting 37

3 Troubleshooting and Test Functions

- Overview of the Pump's Indicators and Test Functions 40
- Status Indicators 41
 - Power Supply Indicator 42
 - Pump Status Indicator 43
- Error Messages 44

Timeout	45
Shut-Down	46
Remote Timeout	47
Synchronization Lost	48
Leak	49
Leak Sensor Open	50
Leak Sensor Short	51
Compensation Sensor Open	52
Compensation Sensor Short	53
Fan Failed	54
Open Cover	55
Restart Without Cover	56
Zero Solvent Counter	57
Pressure Above Upper Limit	58
Pressure Below Lower Limit	59
Pressure Signal Missing	60
Missing Pressure Reading	61
Inlet-Valve Fuse	62
Motor-Drive Power	63
Encoder Missing	64
Inlet-Valve Missing	65
Temperature Out of Range	66
Temperature Limit Exceeded	67
Servo Restart Failed	68
Pump Head Missing	69
Index Limit	70
Index Adjustment	71
Index Missing	72
Stroke Length	73
Initialization Failed	74
Wait Timeout	75
Pressure Test	76

Positioning the blank nut	77
Running the Pressure Test	77
Evaluating the Results	79
Potential Causes of Pressure Test Failure	79
Leak Test	81
Running the Leak Test	83
Evaluating the Results	85

4 Repairing the Pump

Introduction into Repairing the Pump	90
Using the ESD Strap	91
Overview of the Repairing the Pump	92
Simple Repair Procedures	93
Exchanging the Active Inlet Valve	94
Exchanging the Active Inlet Valve Cartridge	96
Exchanging the Outlet Ball Valve	98
Exchanging the Purge Valve Frit or the Purge Valve	100
Removing the Pump Head Assembly	102
Exchanging the Pump Seals and Seal Wear-in Procedure	103
Seal Wear-in Procedure	105
Exchanging the Plungers	106
Installing the Continuous Seal Wash Option	108
Exchanging the Wash Seals	112
Reinstalling the Pump Head Assembly	115
Exchanging the optional Interface Board	116
Exchanging Internal Parts	117
Removing the Top Cover and Foam	118
Exchanging the Low Pressure Pump Main Board (LPM Board)	121
Exchanging the Damper	129
Exchanging the Fan	132

Exchanging the Pump Drive	134
Exchanging the Power Supply	137
Exchanging the Leak Sensor	142
Exchanging the Status Light Pipe	144
Assembling the Main Cover	145
Replacing the Top Cover and Foam	146

5 Parts and Materials

Overview of Main Assemblies	150
Control Module (B-Version)	153
Solvent Cabinet	154
Bottle Head Assembly	155
Hydraulic Path	156
Cover Parts	157
Sheet Metal Kit	158
Foam Parts	159
Power and Status Light Pipes	160
Leak Parts	161
Pump Head Assembly	162
Pump Head Assembly with Seal Wash Option	164
Outlet Ball Valve Assembly	166
Purge Valve Assembly	167
Active Inlet Valve Assembly	168
Accessory Kit G1311-68075	169
Seal Wash Option Kit 01018-68722	170
Cable Overview	171
Analog Cables	173


Remote Cables	176
BCD Cables	181
Auxiliary Cable	183
CAN Cable	184
External Contact Cable	185
RS-232 Cable Kit	186
LAN Cables	187

6 Introduction to the Isocratic Pump

Introduction to the Isocratic Pump	190
Overview	191
How Does the Pump Work?	192
How Does Compressibility Compensation Work?	194
How Does Variable Stroke Volume Work?	195
Electrical Connections	196
Instrument Layout	198
Early Maintenance Feedback (EMF)	199
EMF Counters	199
Using the EMF Counters	200
The Electronics	201
The Low-Pressure Pump Main Board (LPM)	202
Firmware Description	206
Firmware Updates	207
Optional Interface Boards	208
BCD Board	208
LAN Board	209
Agilent 1100 Series Interfaces	211
Analog Signal Output	212
GPIB Interface	212

	CAN Interface	212
	APG Remote Interface	213
	RS-232C	214
	Setting the 8-bit Configuration Switch	216
	GPIB Default Addresses	217
	Communication Settings for RS-232C Communication	218
	Forced Cold-Start Settings	219
	Stay Resident Settings	220
	The Main Power Supply Assembly	221
7	Control Module Screens for the Isocratic Pump	
	Major keys on the Agilent 1100 Control Module	224
	Screens available from the Analysis screen	225
	Screens available from the System screen	234
	Screens available from the Records screen	236
	Diagnostics and Tests	243
8	Specifications	
	Performance Specifications	246
A	Safety Information	
	General Safety Information	250
	Lithium Batteries Information	253
	Radio Interference	254
	Sound Emission	255
	Solvent Information	256
	Agilent Technologies on Internet	257

Index

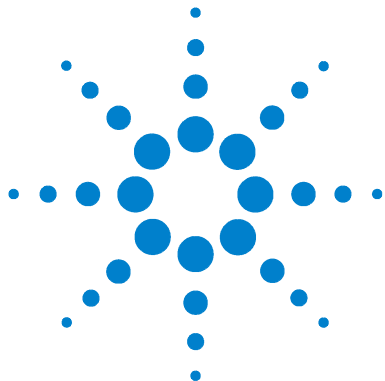

1 Installing the Pump

Site Requirements	12
Unpacking the Isocratic Pump	15
Optimizing the Stack Configuration	17
Installing the Isocratic Pump	19
Flow Connections of the Isocratic Pump	22
Priming and Purging the System	25



Site Requirements

A suitable environment is important to ensure optimum performance of the isocratic pump.

Power Consideration

The isocratic pump power supply has wideranging capability (see [Table 1](#) on page 13). It accepts any line voltage in the range described in the above mentioned table. Consequently there is no voltage selector in the rear of the isocratic pump. There are also no externally accessible fuses, because automatic electronic fuses are implemented in the power supply.

WARNING

To disconnect the isocratic pump from line, unplug the power cord. The power supply still uses some power, even if the power switch on the front panel is turned off.

WARNING

Shock hazard or damage of your instrumentation can result, if the devices are connected to a line voltage higher than specified.

Power Cords

Different power cords are offered as options with the isocratic pump. The female end of each of the power cords is identical. It plugs into the power-input socket at the rear of the isocratic pump. The male end of each of the power cords is different and designed to match the wall socket of a particular country or region.

WARNING

Never operate your instrumentation from a power outlet that has no ground connection. Never use a power cord other than the power cord designed for your region.

WARNING

Never use cables other than the ones supplied by Agilent Technologies to ensure proper functionality and compliance with safety or EMC regulations.

Bench Space

The isocratic pump dimensions and weight (see [Table 1](#)) allow to place the isocratic pump on almost any laboratory bench. It needs an additional 2.5 cm (1.0 inches) of space on either side and approximately 8 cm (3.1 inches) in the rear for the circulation of air and electric connections.

If the bench should carry a complete Agilent 1100 Series system, make sure that the bench is designed to carry the weight of all the modules.

NOTE

The pump should be operated in a horizontal position!

Environment

Your isocratic pump will work within specifications at ambient temperatures and relative humidity as described in [Table 1](#).

CAUTION

Do not store, ship or use your isocratic pump under conditions where temperature fluctuations could cause condensation within the isocratic pump. Condensation will damage the system electronics. If your isocratic pump was shipped in cold weather, leave it in its box and allow it to warm slowly to room temperature to avoid condensation.

Table 1 Physical Specifications

Type	Specification	Comments
Weight	11 kg (25 lbs)	
Dimensions (height × weight × depth)	140 × 345 × 435 mm (5.5 × 13.5 × 17 inches)	
Line voltage	100 – 120 or 220 – 240 VAC, ± 10 %	Wide-ranging capability
Line frequency	50 or 60 Hz, ± 5 %	

1 Installing the Pump

Table 1 Physical Specifications (continued)

Power consumption	220 VA	Maximum
Ambient operating temperature	4 – 55 °C (41 – 131 °F)	
Ambient non-operating temperature	-40 – 70 °C (-4 – 158 °F)	
Humidity	< 95 %, at 25 – 40 °C (77 – 104 °F)	Non-condensing
Operating Altitude	Up to 2000 m (6500 ft)	
Non-operating altitude	Up to 4600 m (14950 ft)	For storing the isocratic pump
Safety standards: IEC, CSA, UL	Installation Category II, Pollution Degree 2	

Unpacking the Isocratic Pump

Damaged Packaging

Upon receipt of your isocratic pump, inspect the shipping containers for any signs of damage. If the containers or cushioning material are damaged, save them until the contents have been checked for completeness and the isocratic pump has been mechanically and electrically checked. If the shipping container or cushioning material is damaged, notify the carrier and save the shipping material for the carrier's inspection.

CAUTION

If there are signs of damage to the isocratic pump, please do not attempt to install the isocratic pump.

Delivery Checklist

Ensure all parts and materials have been delivered with the isocratic pump. The delivery checklist is shown in [Table 2](#). To aid in parts identification, please see [Chapter 5](#), "Parts and Materials. Please report missing or damaged parts to your local Agilent Technologies sales and service office.

Table 2 Isocratic Pump Checklist

Description	Quantity
Isocratic pump	1
Solvent cabinet	1 (5062-8581)
Amber solvent bottle	1 (9301-1450)
Bottle-head assembly	1 (G1311-60003)
Waste tube, purge valve	1 (5042-2461, reorder number, 5m)
Power cable	1
CAN cable, 1 m	1
Remote cable	As ordered

Table 2 Isocratic Pump Checklist (continued)

Description	Quantity
Signal cable	As ordered
<i>Reference Manual</i>	1
Accessory kit (see Table 3)	1

Accessory Kit Contents - Isocratic Pump

Table 3 Accessory Kit Contents G1311-68705

Description	Part Number	Quantity
Capillary, pump to injection device	G1312-67305	1
Seal insert tool	01018-23702	1
Wrench; 1/4 – 5/16 inch	8710-0510	1
Wrench; 14 mm	8710-1924	1
ESD wrist strap*	9300-1408	1
Hex key 4mm	8710-2392	1
Waste tube (reorder number, 5m)	5062-2463	1.2 m
Velocity regulator (reorder number)	5062-2486	2
PTFE Frit	01018-22707	5

* ESD: Electrostatic Discharge

Optimizing the Stack Configuration

If your isocratic pump is part of a complete 1100 Series system, you can ensure optimum performance by limiting the configuration of the system stack to the following configuration. This configuration optimizes the system flow path, ensuring minimum delay volume.

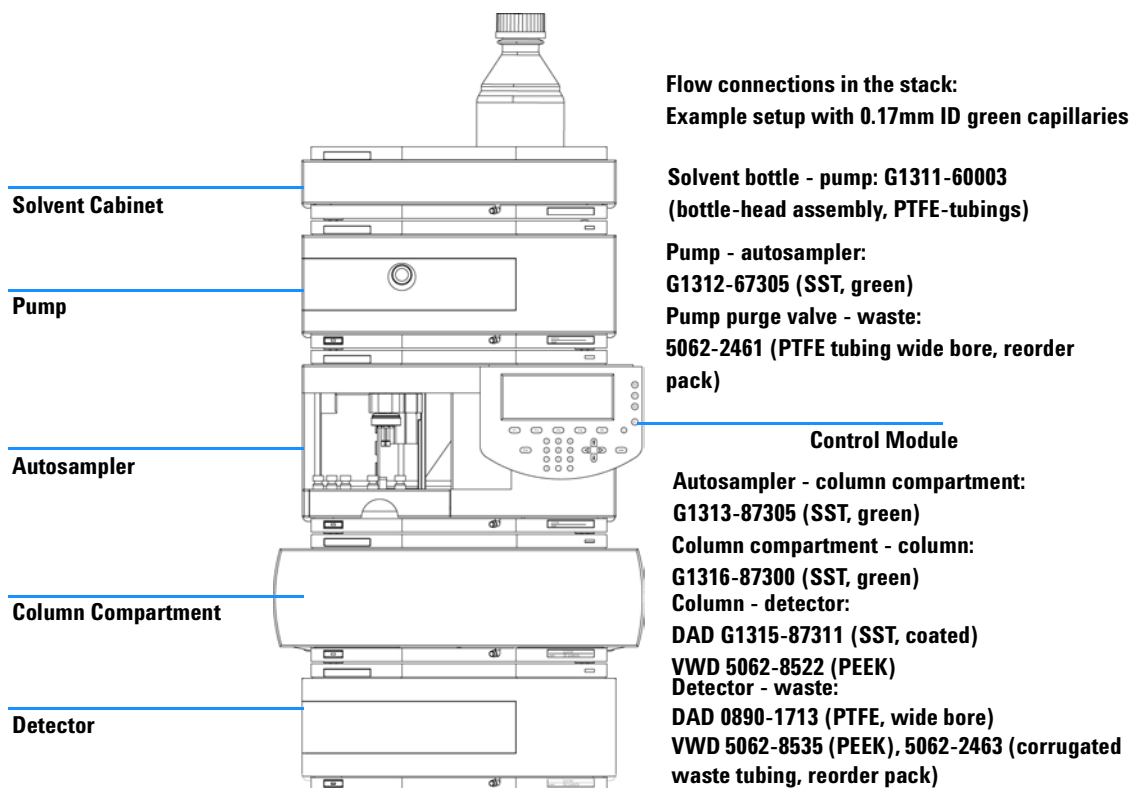


Figure 1 Recommended Stack Configuration (Front View).

NOTE

For a detailed view of the flow connections refer to the section “Flow Connections” in chapter 1 of the reference manuals of the individual modules.

1 Installing the Pump

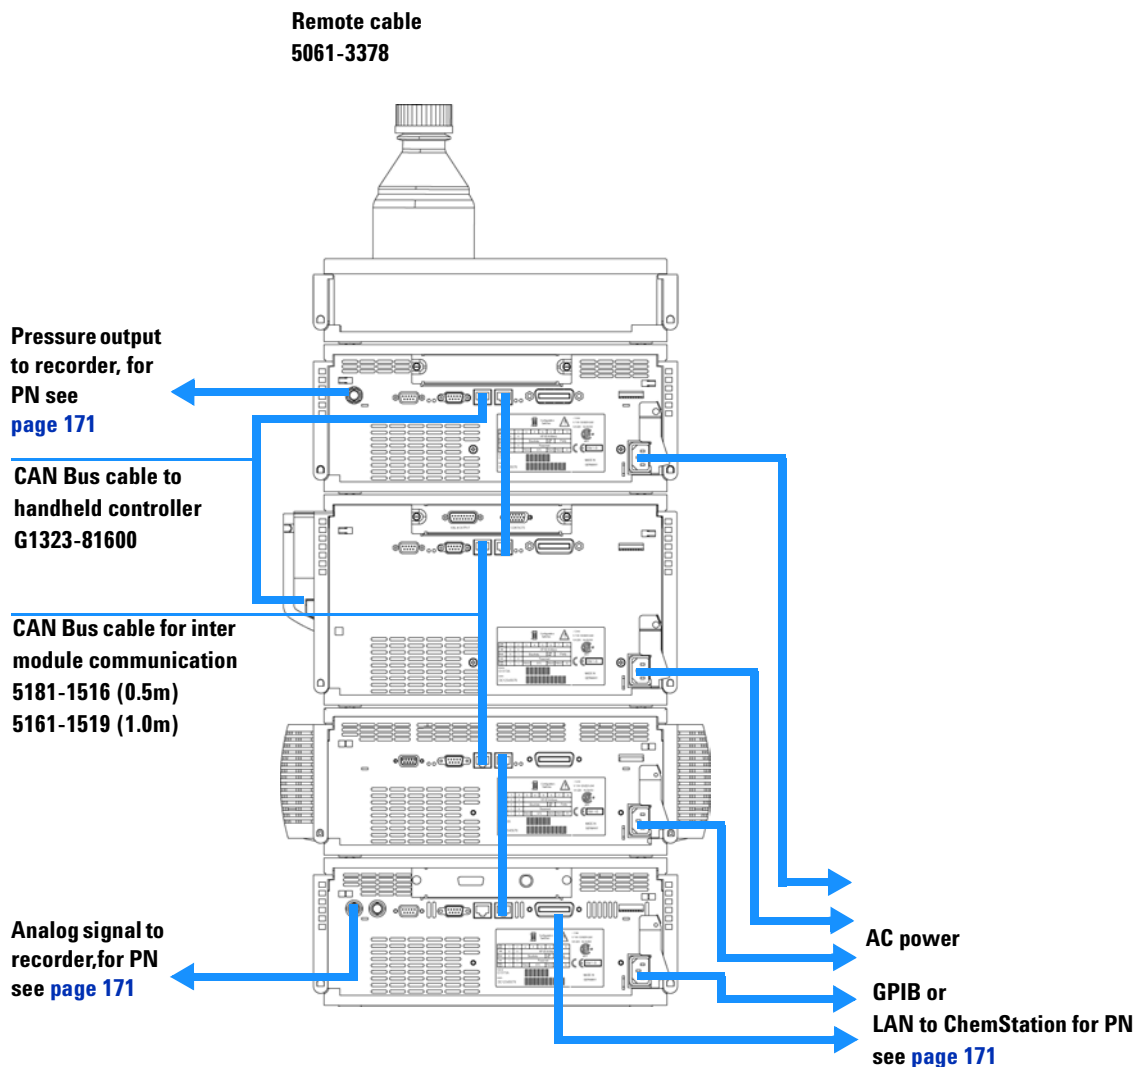


Figure 2 Recommended Stack Configuration (Rear View)

NOTE

If a single stack configuration becomes too high, e.g. if an additional module like a G1327A ALS Thermostat is added or if your bench is too high, a two stack configuration may be a better setup. Separate the stack between pump and autosampler and place the stack containing the pump on the right side of the stack containing the autosampler.

Installing the Isocratic Pump

Preparations	Locate bench space. Provide power connections. Unpack the pump.
Parts required	Pump Power cord, for other cables see text below and see "Cable Overview" on page 171 ChemStation and/or Control Module G1323A/B

- 1 Place the isocratic pump on the bench in a horizontal position.
- 2 Ensure the power switch on the front of the isocratic pump is OFF (switch stands out).

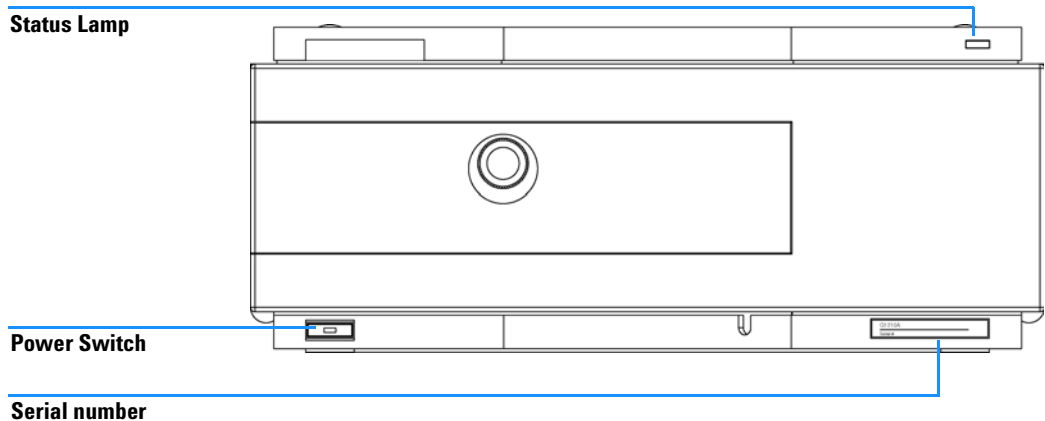


Figure 3 Front of Isocratic Pump

- 3 At the rear of the isocratic pump move the security lever to its maximum right position.
- 4 Connect the power cable to the power connector at the rear of the isocratic pump. The security lever will prevent that the cover is opened while the power cord is connected to the isocratic pump.
- 5 Connect the required interface cables to the rear of the isocratic pump.

1 Installing the Pump

NOTE

In an Agilent 1100 Series system, the individual modules are connected through CAN cables. The Agilent 1100 Series vacuum degasser is an exception. A vacuum degasser can be connected via the APG remote connector to the other modules of the stack. The AUX output allows the user to monitor the vacuum level in the degasser chamber. An Agilent 1100 Series control module can be connected to the CAN bus at any of the modules in the system except for the degasser. The Agilent ChemStation can be connected to the system through one GPIB or LAN (requires the installation of a LAN- board) cable at any of the modules (except for the degasser), preferably at the detector (MUST for the DAD). For more information about connecting the control module or Agilent ChemStation refer to the respective user manual. For connecting the Agilent 1100 Series equipment to non-Agilent 1100 Series equipment, see [Chapter 6](#), "Introduction to the Isocratic Pump."

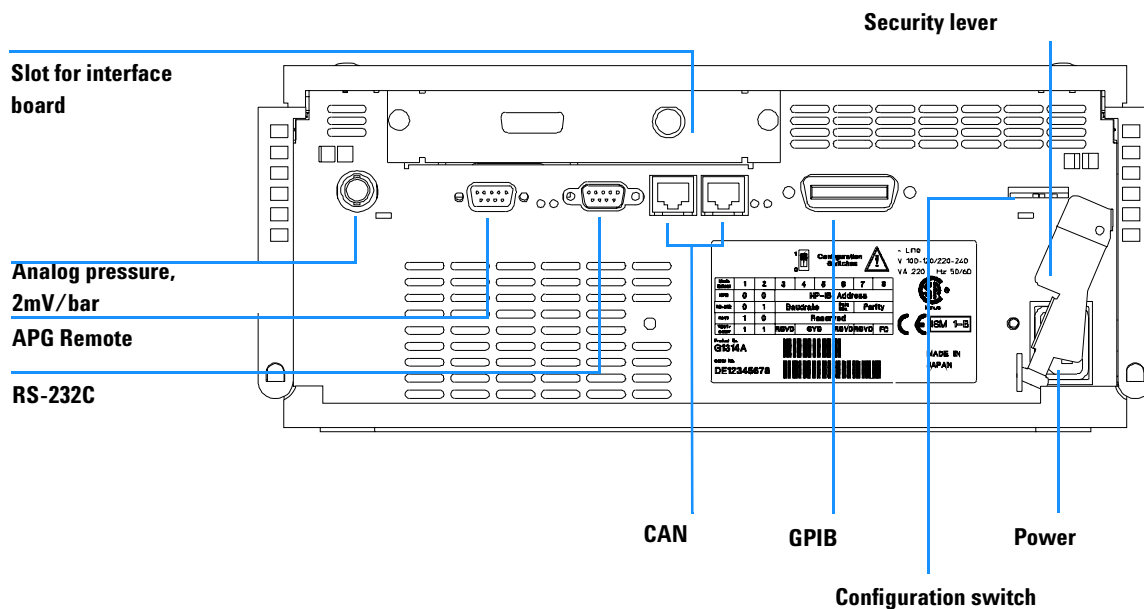


Figure 4 Electrical Connections

- 6 Connect the capillary, solvent tube and waste tubing (see [Figure](#) on page 22).
- 7 Press in the power switch to turn on the isocratic pump.

NOTE

The power switch stays pressed in and a green indicator lamp in the power switch is on when the pump is turned on. When the line power switch stands out and the green light is off, the pump is turned off.

- 8 Purge the isocratic pump (see see [“Priming and Purging the System”](#) on page 25).

WARNING

To disconnect the isocratic pump from line, unplug the power cord. The power supply still uses some power, even if the power switch on the front panel is turned off.

NOTE

The pump was shipped with default configuration settings. To change these settings, see [“Setting the 8-bit Configuration Switch”](#) on page 216

Flow Connections of the Isocratic Pump

WARNING

When opening capillary or tube fittings solvents may leak out. Please observe appropriate safety procedures (for example, goggles, safety gloves and protective clothing) as described in the material handling and safety data sheet supplied by the solvent vendor, especially when toxic or hazardous solvents are used

Preparations Parts required

Pump is installed in the LC system.
Other modules
Parts from accessory kit, see ["Accessory Kit Contents - Isocratic Pump"](#) on page 16
Two wrenches 1/4–5/16 inch for capillary connections

- 1 Remove the front cover by pressing the snap fasteners on both sides.

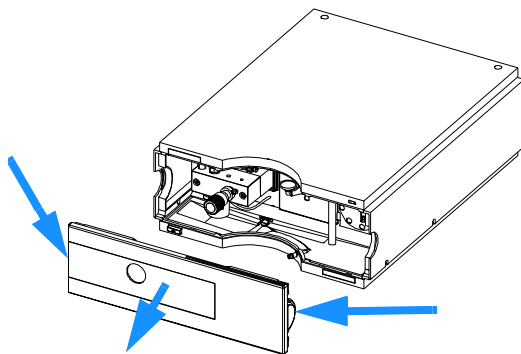


Figure 5 Removing the Front Cover

- 2 Place the solvent cabinet on top of the isocratic pump.
- 3 Place the bottle containing your solvent into the solvent cabinet and place the bottle-head assembly into the bottle.
- 4 Connect the solvent tube from the bottle-head assembly to the inlet adapter of the active inlet valve. Fix the tube in the clips of solvent cabinet and isocratic pump.

- 5 Using a piece of sanding paper connect the waste tubing to the purge valve and place it into your waste system.
- 6 If the isocratic pump is not part of a Agilent1100 System stack or placed on the bottom of a stack, connect the corrugated waste tube to the waste outlet of the pump leak handling system.
- 7 Connect the outlet capillary (isocratic pump to injection device) to the outlet of the purge valve.
- 8 Purge your system before first use (see [“Priming and Purging the System”](#) on page 25).

1 Installing the Pump

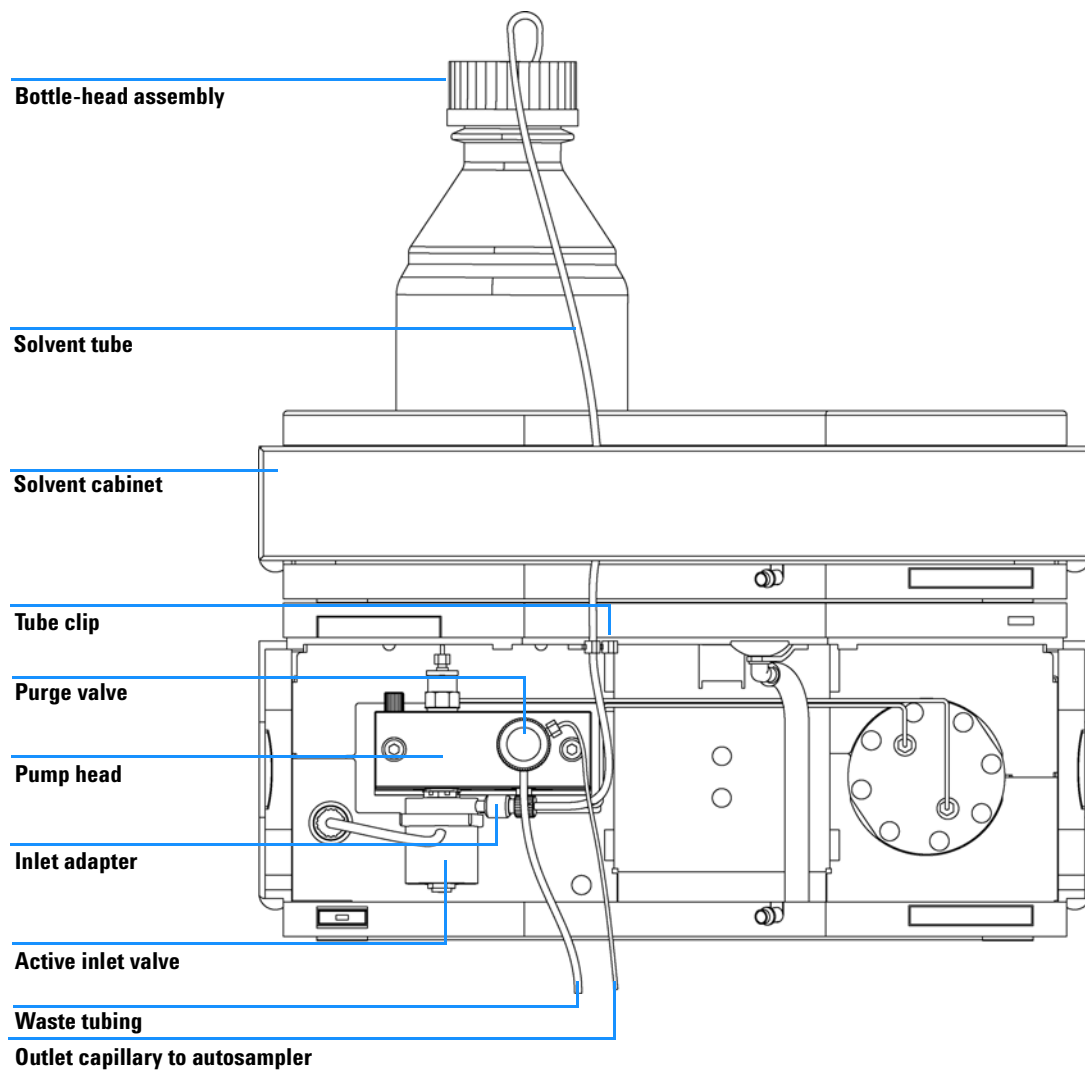


Figure 6 Flow Connections of the Isocratic Pump

Priming and Purging the System

If a degasser is installed, it can be primed either by drawing solvent through the degasser with a syringe or by pumping with the pump.

Priming the vacuum degasser or system with a syringe is recommended, when:

- vacuum degasser or system is used for the first time, or vacuum tubes are empty, or
- changing to solvents that are immiscible with the solvent currently in the tubes.

Priming the system by using the pump at high flow rate (3–5 ml/min) is recommended, when:

- pumping system was turned off for a length of time (for example, overnight) and if volatile solvent mixtures are used, or
- solvents have been changed.

WARNING

When opening capillary or tube fittings solvents may leak out. Please observe appropriate safety procedures (for example, goggles, safety gloves and protective clothing) as described in the material handling and safety data sheet supplied by the solvent vendor, especially when toxic or hazardous solvents are used.

Priming with a Syringe

Before using a new degasser or new tubings for the first time:

- 1 Prime all tubings with at least 30 ml of iso-propanol no matter whether the channel will be used with organic mobile phase or with water.

If you are changing to a solvent that is immiscible with the solvent currently in the tubing continue as follows:

- 2 Replace the current solvent with adequate organic solvent (see [Table 4](#) on page 27), if current solvent is organic or with water, if current solvent is an inorganic buffer or contains salt.
- 3 Disconnect solvent tube from your pump.
- 4 Connect syringe adapter to solvent tube.

1 Installing the Pump

- 5 Push syringe adapter onto syringe.
- 6 Pull syringe plunger to draw at least 30 ml of solvent through degasser and tubing.
- 7 Replace the priming solvent with the new solvent of your choice.
- 8 Pull syringe plunger to draw at least 30 ml of solvent through degasser and tubing.
- 9 Disconnect syringe adapter from solvent tube.
- 10 Connect solvent tube to your pump.

NOTE

When priming the vacuum degasser with a syringe the solvent is drawn through the degasser tubes very quickly. The solvent at the degasser outlet will therefore not be fully degassed. Pump for approximately 10 minutes with your selected flow rate before starting any application. This will allow the vacuum degasser to properly degas the solvent in the degasser tubes.

NOTE

The pump should never be used for priming empty tubings (never let the pump run dry). Use the syringe to draw enough solvent for completely filling the tubings to the pump inlet before continuing to prime with the pump.

Priming with the Pump

When the pumping system has been turned off for a certain time (for example, overnight) oxygen will rediffuse into the solvent channel between the vacuum degasser and the pump. Solvents containing volatile ingredients will slightly lose these, if left in the degasser without flow for a prolonged period of time. Therefore priming of the vacuum degasser and the pumping system is required before starting an application.

- 1 Open the purge valve of your pump (by turning it counterclockwise) and set flow rate to 3-5 ml/min.
- 2 Flush the vacuum degasser and all tubes with at least 30 ml of solvent.
- 3 Set flow to required value of your application and close the purge valve.
- 4 Pump for approximately 10 minutes before starting your application.

Table 4 Choice of Priming Solvents for Different Purposes

Activity	Solvent	Comments
After an installation	Isopropanol	Best solvent to flush air out of the system
When switching between reverse phase and normal phase (both times)	Isopropanol	Best solvent to flush air out of the system
After an installation	Ethanol or Methanol	Alternative to Isopropanol (second choice) if no Isopropanol is available
To clean the system when using buffers	Bidistilled water	Best solvent to re-dissolve buffer crystals
After a solvent change	Bidistilled water	Best solvent to re-dissolve buffer crystals
After the installation of normal phase seals (P/N 0905-1420)	Hexane + 5% Isopropanol	Good wetting properties

1 Installing the Pump



2 Optimizing Performance

Hints for Successful Use of the Isocratic Pump	30
Solvent Information	31
Prevent Blocking of Solvent Filters	32
When to Use a Vacuum Degasser	34
When to use the Continuous Seal Wash Option	35
When to Use Alternative Seals	36
How to Optimize the Compressibility Compensation Setting	37




Hints for Successful Use of the Isocratic Pump

- Always place solvent cabinet with the solvent bottle on top of the isocratic pump (or at a higher level).
- When using the isocratic pump without vacuum degasser, shortly degass your solvents. Vacuum pump the solvents for 15 – 30 s (in an appropriate vessel) before using them in the isocratic pump. If possible apply solvent conditions that will decrease the gas solubility (for example, warming up the solvents).
- For highest precision and reproducibility use vacuum degasser.
- When using the isocratic pump with vacuum degasser – before operating the isocratic pump flush the degasser with at least two volumes (30 ml), especially when turned off for a certain length of time (for example, during the night) and volatile solvent mixtures are used in the channels (see [“Priming and Purging the System”](#) on page 25).
- Prevent blocking of solvent inlet filters (never use the pump without solvent inlet filter). Growth of algae should be avoided (see [“Prevent Blocking of Solvent Filters”](#) on page 32).
- Check purge valve frit and column frit in regular time intervals. A blocked purge valve frit can be identified by black or yellow layers on its surface or by a pressure greater than 10 bar, when pumping distilled water at a rate of 5 ml/min with an open purge valve.
- When using the isocratic pump at low flow rates (for example, 0.2 ml/min) check all 1/16 inch fittings for any signs of leaks.
- Always exchange the purge valve frit, too, when exchanging the seals.
- When using buffer solutions, flush the system with water before switching it off. The seal wash option should be used when buffer solutions of 0.1 Molar or higher will be used for long time periods.
- Check the pump plungers for scratches when changing the plunger seals. Scratched plungers will lead to micro leaks and will decrease the lifetime of the seal.
- After changing plunger seals apply the seal wear-in procedure (see [“Exchanging the Pump Seals and Seal Wear-in Procedure”](#) on page 103).

Solvent Information

Always filter solvents through 0.4 µm filters, small particles can permanently block the capillaries and valves. Avoid the use of the following steel-corrosive solvents:

- Solutions of alkali halides and their respective acids (for example, lithium iodide, potassium chloride, and so on).
- High concentrations of inorganic acids like sulfuric acid, especially at higher temperatures (replace, if your chromatography method allows, by phosphoric acid or phosphate buffer which are less corrosive against stainless steel).
- Halogenated solvents or mixtures which form radicals and/or acids, for example:



This reaction, in which stainless steel probably acts as a catalyst, occurs quickly with dried chloroform if the drying process removes the stabilizing alcohol.

- Chromatographic grade ethers, which can contain peroxides (for example, THF, dioxane, di-isopropylether) such ethers should be filtered through dry aluminium oxide which adsorbs the peroxides.
- Mixtures of carbon tetrachloride with 2-propanol or THF dissolve stainless steel.

Prevent Blocking of Solvent Filters

Contaminated solvents or algae growth in the solvent bottle will reduce the lifetime of the solvent filter and will influence the performance of the isocratic pump. This is especially true for aqueous solvents or phosphate buffers (pH 4 to 7). The following suggestions will prolong lifetime of the solvent filter and will maintain the performance of the isocratic pump.

- Use a sterile, if possible amber, solvent bottle to slow down algae growth.
- Filter solvents through filters or membranes that remove algae.
- Exchange solvents every two days or refilter.
- If the application permits add 0.0001-0.001M sodium azide to the solvent.
- Place a layer of argon on top of your solvent.
- Avoid exposure of the solvent bottle to direct sunlight.

Checking the Solvent Filter

The solvent filter is located on the low-pressure side of the isocratic pump. A blocked filter therefore does not affect the pressure readings of the isocratic pump. The pressure readings cannot be used to check whether the filter is blocked or not. If the solvent cabinet is placed on top of the pump the filter condition can be checked in the following way:

Remove solvent inlet tube from the adapter at the AIV. If the filter is in good condition the solvent will freely drip out of the solvent tube (hydrostatic pressure). If the solvent filter is partly blocked only very little solvent will drip out of the solvent tube.

Cleaning the Solvent Filter

- Remove the blocked solvent filter from the bottle-head assembly and place it in a beaker with concentrated nitric acid (35%) for one hour.
- Thoroughly flush the filter with bidistilled water (remove all nitric acid, some capillary columns can be damaged by nitric acid).
- Replace the filter.

NOTE

Never use the system without solvent filter installed.

When to Use a Vacuum Degasser

The isocratic pump does not necessarily require degassing. But for the following conditions the vacuum degasser is recommended:

- if your detector is used with maximum sensitivity in the low UV wavelength range,
- if your application requires highest injection precision, or
- if your application requires highest retention-time reproducibility (mandatory at flow rates below 0.5 ml/min).

Operational Hints for the Vacuum Degasser

If you are using the vacuum degasser for the first time, if the vacuum degasser was switched off for any length of time (for example, overnight), or if the vacuum degasser lines are empty, you should prime the vacuum degasser before running an analysis.

The vacuum degasser can be primed either by drawing solvent through the degasser with a syringe or by pumping with the isocratic pump.

Priming the degasser with a syringe is recommended, when:

- vacuum degasser is used for the first time, or vacuum tubes are empty, or
- changing to solvents that are immiscible with the solvent currently in the vacuum tubes.

Priming the vacuum degasser by using the isocratic pump at high flow rate is recommended, when:

- isocratic pump was turned off for a length of time (for example, during night) and volatile solvent mixtures are used, or
- solvents have been changed.

For more information see the *Reference Manual* for the Agilent 1100 Series vacuum degasser.

When to use the Continuous Seal Wash Option

Highly-concentrated buffer solutions will reduce the lifetime of the seals and plungers in your isocratic pump. The seal wash option allows to maintain the seal lifetime by flushing the back side of the seal with a wash solvent.

The continuous seal wash option is strongly recommended when buffer concentrations of 0.1 Molar or higher will be used for long time periods in the isocratic pump.

The continuous seal wash option can be ordered by quoting part number 01018-68722 (kit contains all parts needed for one pump head).

The seal wash option comprises a support ring, secondary seal, gasket and seal keeper for both plunger sides. A wash bottle filled with water /isopropanol (90/10) should be placed above the isocratic pump in the solvent cabinet and gravity will maintain a flow through the pump head removing all possible buffer crystals from the back of the pump seal.

NOTE

Running dry is the worst case for a seal and drastically reduces its lifetime.

The seal will build up sticky layers on the surface of the plunger. These sticky layers will also reduce the lifetime of the primary seal. Therefore the tubes of the wash option should always be filled with solvent to prolong the lifetime of the wash seal. Always use a mixture of bidistilled water (90 %) and isopropanol (10 %) as wash solvent. This mixture prevents bacteria growth in the wash bottle and reduces the surface tension of the water. The flow rate should be regulated to approximately 20 drops/minute. This can be done with the velocity regulator supplied with the accessory kit

For information on the installation of the continuous seal wash option refer to "[Installing the Continuous Seal Wash Option](#)" on page 108.

When to Use Alternative Seals

The standard seal for the isocratic pump can be used for most applications. However applications that use normal phase solvents (for example, hexane) are not suited for the standard seal and require a different seal when used for a longer time in the isocratic pump.

For applications that use normal phase solvents (for example, hexane) we recommend the use of the polyethylene seals, Agilent Technologies part number 0905-1420 (pack of 2). These seals have less abrasion compared to the standard seals.

NOTE

Polyethylene seals have a limited pressure range 0–200 bar. When used above 200 bar their lifetime will be significantly reduced. **DO NOT** apply the seal wear-in procedure performed with new standard seals at 400 bar.

How to Optimize the Compressibility Compensation Setting

The compressibility compensation default setting is 100×10^{-6} /bar for the isocratic pump. This setting represents an average value. Under normal conditions the default setting reduces the pressure pulsation (ripple) to values (below 1 % of system pressure) that will be sufficient for most applications. For applications using sensitive detectors, the compressibility settings can be optimized by using the values for various solvents described in Table 5 on page 41. If the solvent in use is not listed in the compressibility tables, when using mixtures of solvents and if the default settings are not sufficient for your application, the following procedure can be used to optimize the compressibility settings:

- 1 Start the isocratic pump with the required flow rate.
- 2 Before starting the optimization procedure, the flow must be stable. Use degassed solvent only. Check the tightness of the system with the pressure test (see "Pressure Test" on page 76).
- 3 Your pump must be connected to a Chemstation or handheld controller, the pressure and %-ripple can be monitored with one of these instruments,

otherwise connect a signal cable between the pressure output of the isocratic pump and a recording device (for example, 339X integrator) and set parameters.

Zero 50 %

Att 2³

Chart Speed 10 cm/min

- 4 Start the recording device with the plot mode.
- 5 Starting with a compressibility setting of 10×10^{-6} /bar increase the value in steps of 10. Re-zero the integrator as required. The compressibility compensation setting that generates the smallest pressure ripple is the optimum value for your solvent composition.

2 Optimizing Performance

Table 5 Solvent Compressibility

Solvent (pure)	Compressibility ($10^{-6}/\text{bar}$)
Acetone	126
Acetonitrile	115
Benzene	95
Carbon tetrachloride	110
Chloroform	100
Cyclohexane	118
Ethanol	114
Ethyl acetate	104
Heptane	120
Hexane	150
Isobutanol	100
Isopropanol	100
Methanol	120
1-Propanol	100
Toluene	87
Water	46



3 Troubleshooting and Test Functions

Overview of the Pump's Indicators and Test Functions 40

Status Indicators 41

Error Messages 44

Pressure Test 76

Leak Test 81



Overview of the Pump's Indicators and Test Functions

Status Indicators

The isocratic pump is provided with two status indicators which indicate the operational state (prerun, run, and error states) of the isocratic pump. The status indicators provide a quick visual check of the operation of the isocratic pump (see [“Status Indicators”](#) on page 41).

Error Messages

In the event of an electronic, mechanical or hydraulic failure, the isocratic pump generates an error message in the user interface. The following pages describe the meaning of the error messages. For each message, a short description of the failure, a list of probable causes of the problem, and a list of suggested actions to fix the problem are provided (see [“Error Messages”](#) on page 44).

Pressure Test

The pressure test is a quick test designed to determine the pressure tightness of the system. After exchanging flow path components (e.g. pump seals or injection seal), use this test to verify the system is pressure tight up to 400 bar (see [“Pressure Test”](#) on page 76).

Leak Test

The leak test is a diagnostic test designed to determine the pressure tightness of the isocratic pump. When a problem with the isocratic pump is suspected, use this test to help troubleshoot the isocratic pump and its pumping performance. The following sections describe these functions in detail (see [“Leak Test”](#) on page 81).

Status Indicators

Two status indicators are located on the front of the isocratic pump. The lower left one indicates the power supply status, the upper right one indicates the isocratic pump status.

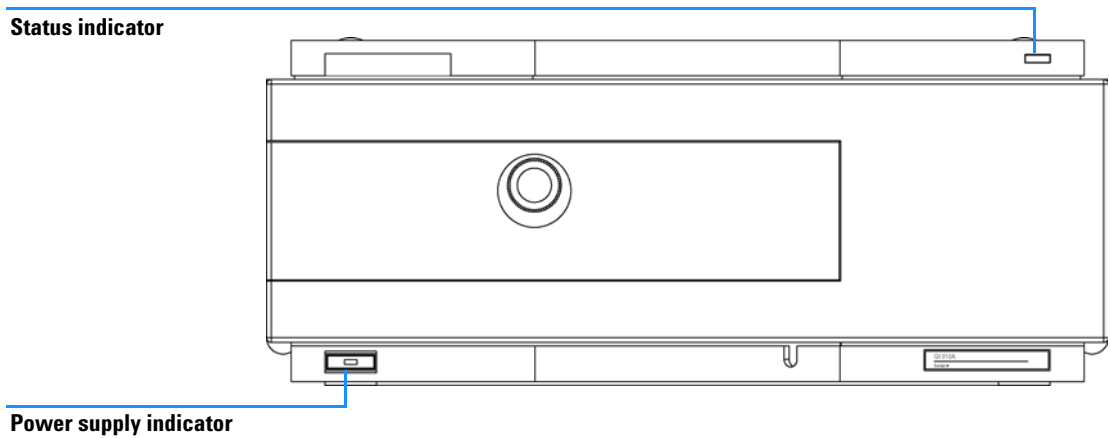


Figure 7 Location of Status Indicators

Power Supply Indicator

The power supply indicator is integrated into the main power switch. When the indicator is illuminated (*green*) the power is ON.

When the indicator is off, the module is turned OFF. Otherwise check power connections, availability of power or check functioning of the power supply.

Pump Status Indicator

The Pump status indicator indicates one of four possible instrument conditions:

- When the status indicator is *OFF* (and power switch light is on), the isocratic pump is in a *prerun* condition, and is ready to begin an analysis.
- A *green* status indicator, indicates the isocratic pump is performing an analysis (*run* mode).
- A *yellow* indicator indicates a *not-ready* condition. The isocratic pump is in a not-ready state when it is waiting for a specific condition to be reached or completed (for example, immediately after changing a setpoint), or while a self-test procedure is running.
- An *error* condition is indicated when the status indicator is *red*. An error condition indicates the isocratic pump has detected an internal problem which affects correct operation of the isocratic pump. Usually, an error condition requires attention (for example, leak, defective internal components). An error condition always interrupts the analysis.
- A *flashing yellow* status indicator indicates that the module is in its *resident mode*. Call your local service provider for assistance upon observing this error condition.
- A *flashing red* status indicator indicates a severe error during the *startup* procedure of the module. Call your local service provider for assistance upon observing this error condition.

Error Messages

Error messages are displayed in the user interface when an electronic, mechanical, or hydraulic (flow path) failure occurs which requires attention before the analysis can be continued (for example, repair, frit exchange or exchange of consumables required). In the event of such a failure, the red status indicator at the front of the isocratic pump is switched on, and an entry is written into the instrument logbook.

Timeout

The timeout threshold was exceeded.

Probable Causes

- The analysis was completed successfully, and the timeout function switched off the isocratic pump as requested.
- A not-ready condition was present during a sequence or multiple-injection run for a period longer than the timeout threshold.

Suggested Actions

- ✓ Check the logbook for the occurrence and source of a not-ready condition. Restart the analysis where required.

Shut-Down

An external instrument has generated a shut-down signal on the remote line.

The isocratic pump continually monitors the remote input connectors for status signals. A LOW signal input on pin 4 of the remote connector generates the error message.

Probable Causes

- Leak detected in another module with a CAN connection to the system .
- Leak detected in an external instrument with a remote connection to the system.
- Shut-down in an external instrument with a remote connection to the system.
- The degasser failed to generate sufficient vacuum for solvent degassing.

Suggested Actions

- ✓ Fix the leak in the external instrument before restarting the isocratic pump.
- ✓ Check external instruments for a shut-down condition.
- ✓ Check the vacuum degasser for an error condition. Refer to the *Reference Manual* for the Agilent 1100 Series vacuum degasser.

Remote Timeout

A not-ready condition is still present on the remote input .

When an analysis is started, the system expects all not-ready conditions (e.g. a not-ready condition during detector balance) to switch to run conditions within one minute of starting the analysis. If a not-ready condition is still present on the remote line after one minute the error message is generated.

Probable Causes

- Not-ready condition in one of the instruments connected to the remote line.
- Defective remote cable.
- Defective components in the instrument showing the not-ready condition.

Suggested Actions

- ✓ Ensure the instrument showing the not-ready condition is installed correctly, and is set up correctly for analysis.
- ✓ Exchange the remote cable.
- ✓ Check the instrument for defects (refer to the instrument's reference documentation).

Synchronization Lost

During an analysis, the internal synchronization or communication between one or more of the modules in the system has failed.

The system processors continually monitor the system configuration. If one or more of the modules is no longer recognized as being connected to the system, the error message is generated.

Probable Causes

- CAN cable disconnected.
- Defective CAN cable.
- Defective main board in another module.

Suggested Actions

- ✓ Ensure all the CAN cables are connected correctly.
- ✓ Switch off the system. Restart the system, and determine which module or modules are not recognized by the system.
- ✓ Ensure all CAN cables are installed correctly.

Leak

A leak was detected in the isocratic pump.

The signals from the two temperature sensors (leak sensor and board-mounted temperature-compensation sensor) are used by the leak algorithm to determine whether a leak is present. When a leak occurs, the leak sensor is cooled by the solvent. This changes the resistance of the leak sensor which is sensed by the leak-sensor circuit on the LPM board

Probable Causes

- Loose fittings.
- Broken capillary.
- Loose or leaking purge valve, active inlet valve, or outlet ball valve.
- Defective pump seals.

Suggested Actions

- ✓ Ensure all fittings are tight.
- ✓ Exchange defective capillaries.
- ✓ Ensure pump components are seated correctly. If there are still signs of a leak, exchange the appropriate seal (purge valve, active inlet valve, outlet ball valve).
- ✓ Exchange the pump seals.

Leak Sensor Open

The leak sensor in the isocratic pump has failed (open circuit).

The current through the leak sensor is dependent on temperature. A leak is detected when solvent cools the leak sensor, causing the leak-sensor current to change within defined limits. If the current falls outside the lower limit, the error message is generated.

Probable Causes

- Leak sensor not connected to the LPM board.
- Defective leak sensor.
- Leak sensor incorrectly routed, being pinched by a metal component.

Suggested Actions

- ✓ Ensure the leak sensor is connected correctly.
- ✓ Exchange the leak sensor.

Leak Sensor Short

The leak sensor in the isocratic pump has failed (short circuit).

The current through the leak sensor is dependent on temperature. A leak is detected when solvent cools the leak sensor, causing the leak-sensor current to change within defined limits. If the current increases above the upper limit, the error message is generated.

Probable Causes

- Defective leak sensor.
- Leak sensor incorrectly routed, being pinched by a metal component.

Suggested Actions

- ✓ Exchange the leak sensor.

Compensation Sensor Open

The ambient-compensation sensor (NTC) on the LPM board in the isocratic pump has failed (open circuit).

The resistance across the temperature compensation sensor (NTC) on the LPM board is dependent on ambient temperature. The change in resistance is used by the leak circuit to compensate for ambient temperature changes. If the resistance across the sensor increases above the upper limit, the error message is generated.

Probable Causes

- Defective LPM board.

Suggested Actions

- ✓ Exchange the LPM board.

Compensation Sensor Short

The ambient-compensation sensor (NTC) on the LPM board in the isocratic pump has failed (short circuit).

The resistance across the temperature compensation sensor (NTC) on the LPM board is dependent on ambient temperature. The change in resistance is used by the leak circuit to compensate for ambient temperature changes. If the resistance across the sensor falls below the lower limit, the error message is generated.

Probable Causes

- Defective LPM board.

Suggested Actions

- ✓ Exchange the LPM board.

Fan Failed

The cooling fan in the isocratic pump has failed.

The hall sensor on the fan shaft is used by the LPM board to monitor the fan speed. If the fan speed falls below 2 revolutions/second for longer than 5 seconds, the error message is generated.

Probable Causes

- Fan cable disconnected.
- Defective fan.
- Defective LPM board.
- Improperly positioned cables or wires obstructing fan blades.

Suggested Actions

- ✓ Ensure the fan is connected correctly.
- ✓ Exchange fan.
- ✓ Exchange the LPM board.
- ✓ Ensure the fan is not mechanically blocked.

Open Cover

The top foam has been removed.

The sensor on the LPM board detects when the top foam is in place. If the foam is removed, the fan is switched off, and the error message is generated.

Probable Causes

- The top foam was removed during operation.
- Foam not activating the sensor.
- Sensor defective.
- Rear of the module is exposed to strong direct sunlight.

Suggested Actions

- ✓ Replace the top foam.
- ✓ Exchange the LPM board.
- ✓ Ensure that the rear of module is not directly exposed to strong sunlight.

Restart Without Cover

The isocratic pump was restarted with the top cover and foam open.

The sensor on the LPM board detects when the top foam is in place. If the isocratic pump is restarted with the foam removed, the isocratic pump switches off within 30 s, and the error message is generated.

Probable Causes

- The isocratic pump started with the top cover and foam removed.
- Rear of the module is exposed to strong direct sunlight.

Suggested Actions

- ✓ Replace the top cover and foam.
- ✓ Ensure that the rear of module is not directly exposed to strong sunlight.

Zero Solvent Counter

Pump firmware version A.02.32 and higher allow to set solvent bottle fillings at the ChemStation (revision 5.xx and higher). If the volume level in the bottle falls below the specified value the error message appears when the feature is configured accordingly.

Probable Causes

- Volume in bottle below specified volume.
- Incorrect setting of limit.

Suggested Actions

- ✓ Refill bottle and reset solvent counter.

Pressure Above Upper Limit

The system pressure has exceeded the upper pressure limit.

Probable Causes

- Upper pressure limit set too low.
- Blockage in the flowpath (after the damper).
- Defective damper.
- Defective LPM board.

Suggested Actions

- ✓ Ensure the upper pressure limit is set to a value suitable for the analysis.
- ✓ Check for blockage in the flowpath. The following components are particularly subject to blockage:
 - purge-valve frit.
 - needle (autosampler),
 - seat capillary (autosampler),
 - sample loop (autosampler), and
 - column frits.
 - capillaries with low internal diameters (e.g. 0.12mm id).
- ✓ Exchange the damper.
- ✓ Exchange the LPM board.

Pressure Below Lower Limit

The system pressure has fallen below the lower pressure limit.

Probable Causes

- Lower pressure limit set too high.
- Air bubbles in the mobile phase.
- Leak.
- Defective damper.
- Defective LPM board.

Suggested Actions

- ✓ Ensure the lower pressure limit is set to a value suitable for the analysis.
- ✓ Ensure solvents are degassed. Purge the isocratic pump.
- ✓ Ensure solvent inlet filters are not blocked.
- ✓ Inspect the pump head, capillaries and fittings for signs of a leak.
- ✓ Purge the isocratic pump. Run a pressure test to determine whether the seals or other pump components are defective.
- ✓ Exchange the damper.
- ✓ Exchange the LPM board.

Pressure Signal Missing

The pressure signal from the damper is missing.

The pressure signal from the damper must be within a specific voltage range. If the pressure signal is missing, the processor detects a voltage of approximately -120mV across the damper connector.

Probable Causes

- Damper disconnected.
- Defective damper.

Suggested Actions

- ✓ Ensure the damper is connected correctly to the LPM board.
- ✓ Exchange the damper.

Missing Pressure Reading

The pressure readings read by the pump ADC (analog-digital converter) are missing.

The ADC reads the pressure readings from the damper every 1ms. If the readings are missing for longer than 10 seconds, the error message is generated.

Probable Causes

- Damper not connected.
- Defective damper.
- Defective LPM board.

Suggested Actions

- ✓ Ensure the damper is connected, clean and seated correctly.
- ✓ Exchange the damper.
- ✓ Exchange the LPM board.

Inlet-Valve Fuse

The active-inlet valve in the isocratic pump has drawn excessive current causing the inlet-valve electronic fuse to open.

Probable Causes

- Defective active inlet valve.
- Defective connection cable (front panel to LPM board).
- Defective LPM board.

Suggested Actions

- ✓ Restart the isocratic pump. If the error message appears again, exchange the active inlet valve.
- ✓ Exchange the connection cable.
- ✓ Exchange the LPM board.

Motor-Drive Power

The current drawn by the pump motor exceeded the maximum limit.

Blockages in the flow path are usually detected by the pressure sensor in the damper, which result in the pump switching off when the upper pressure limit is exceeded. If a blockage occurs before the damper, the pressure increase cannot be detected by the pressure sensor and the isocratic pump will continue to pump. As pressure increases, the pump drive draws more current. When the current reaches the maximum limit, the isocratic pump is switched off, and the error message is generated.

Probable Causes

- Flow path blockage in front of the damper.
- Blocked active inlet valve.
- Blocked outlet ball valve.
- High friction (partial mechanical blockage) in the pump drive assembly.
- Defective pump drive assembly.
- Defective LPM board.

Suggested Actions

- ✓ Ensure the capillaries and frits between the pump head and damper inlet are free from blockage.
- ✓ Exchange the active inlet valve.
- ✓ Exchange the outlet ball valve.
- ✓ Remove the pump-head assembly. Ensure there is no mechanical blockage of the pump-head assembly or pump drive assembly.
- ✓ Exchange the pump drive assembly.
- ✓ Exchange the LPM board.

Encoder Missing

The optical encoder on the pump motor in the isocratic pump is missing or defective.

The processor checks the presence of the pump encoder connector every 2 seconds. If the connector is not detected by the processor, the error message is generated.

Probable Causes

- Defective or disconnected pump encoder connector.
- Defective pump drive assembly.

Suggested Actions

- ✓ Ensure the connector is clean, and seated correctly.
- ✓ Exchange the pump drive assembly.

Inlet-Valve Missing

The active-inlet valve in the isocratic pump is missing or defective.

The processor checks the presence of the active-inlet valve connector every 2 seconds. If the connector is not detected by the processor, the error message is generated.

Probable Causes

- Disconnected or defective cable.
- Disconnected or defective connection cable (front panel to LPM board).
- Defective active inlet valve.

Suggested Actions

- ✓ Ensure the pins of the active inlet valve connector are not damaged. Ensure the connector is seated securely.
- ✓ Ensure the connection cable is seated correctly. Exchange the cable if defective.
- ✓ Exchange the active inlet valve.

Temperature Out of Range

The temperature sensor readings in the motor-drive circuit are out of range.

The values supplied to the ADC by the hybrid sensors must be between 0.5 V and 4.3 V. If the values are outside this range, the error message is generated.

Probable Causes

- Defective LPM board.

Suggested Actions

- ✓ Exchange the LPM board.

Temperature Limit Exceeded

The temperature of one of the motor-drive circuits is too high.

The processor continually monitors the temperature of the drive circuits on the LPM board. If excessive current is being drawn for long periods, the temperature of the circuits increases. If the temperature exceeds the upper limit of 95 °C, the error message is generated.

Probable Causes

- High friction (partial mechanical blockage) in the pump drive assembly.
- Partial blockage of the flowpath in front of the damper.
- Defective pump drive assembly.
- Defective LPM board.

Suggested Actions

- ✓ Ensure the capillaries and frits between the pump head and damper inlet are free from blockage.
- ✓ Ensure the outlet valve is not blocked.
- ✓ Remove the pump head assembly. Ensure there is no mechanical blockage of the pump head assembly or pump drive assembly.
- ✓ Exchange the pump drive assembly.
- ✓ Exchange the LPM board.

Servo Restart Failed

The pump motor in the isocratic pump was unable to move into the correct position for restarting.

When the isocratic pump is switched on, the first step is to switch on the C phase of the variable reluctance motor. The rotor should move to one of the C positions. The C position is required for the servo to be able to take control of the phase sequencing with the commutator. If the rotor is unable to move, or if the C position cannot be reached, the error message is generated.

Probable Causes

- Disconnected or defective cables.
- Blocked active inlet valve.
- Mechanical blockage of the isocratic pump.
- Defective pump drive assembly.
- Defective LPM board.

Suggested Actions

- ✓ Ensure the pump-assembly cables are not damaged or dirty. Make sure the cables are connected securely to the LPM board.
- ✓ Exchange the active inlet valve.
- ✓ Remove the pump-head assembly. Ensure there is no mechanical blockage of the pump-head assembly or pump drive assembly.
- ✓ Exchange the pump drive assembly.
- ✓ Exchange the LPM board.

Pump Head Missing

The pump-head end stop in the isocratic pump was not found.

When the isocratic pump restarts, the metering drive moves forward to the mechanical end stop. Normally, the end stop is reached within 20 seconds, indicated by an increase in motor current. If the end point is not found within 20 seconds, the error message is generated.

Probable Causes

- Pump head not installed correctly (screws not secured, or pump head not seated correctly).
- Broken plunger.

Suggested Actions

- ✓ Install the pump head correctly. Ensure nothing (e.g. capillary) is trapped between the pump head and body.
- ✓ Exchange the plunger.

Index Limit

The time required by the plunger to reach the encoder index position was too short (isocratic pump).

During initialization, the first plunger is moved to the mechanical stop. After reaching the mechanical stop, the plunger reverses direction until the encoder index position is reached. If the index position is reached too fast, the error message is generated.

Probable Causes

- Irregular or sticking drive movement.
- Defective pump drive assembly.

Suggested Actions

- ✓ Remove the pump head, and examine the seals, plungers, and internal components for signs of wear, contamination or damage. Exchange components as required.
- ✓ Exchange the pump drive assembly.

Index Adjustment

The encoder index position in the isocratic pump is out of adjustment.

During initialization, the first plunger is moved to the mechanical stop. After reaching the mechanical stop, the plunger reverses direction until the encoder index position is reached. If the time to reach the index position is too long, the error message is generated.

Probable Causes

- Irregular or sticking drive movement.
- Defective pump drive assembly.

Suggested Actions

- ✓ Remove the pump head, and examine the seals, plungers, and internal components for signs of wear, contamination or damage. Exchange components as required.
- ✓ Exchange the pump drive assembly.

Index Missing

The encoder index position in the isocratic pump was not found during initialization.

During initialization, the first plunger is moved to the mechanical stop. After reaching the mechanical stop, the plunger reverses direction until the encoder index position is reached. If the index position is not recognized within a defined time, the error message is generated.

Probable Causes

- Disconnected or defective encoder cable.
- Defective pump drive assembly.

Suggested Actions

- ✓ Ensure the encoder cable are not damaged or dirty. Make sure the cables are connected securely to the LPM board.
- ✓ Exchange the pump drive assembly.

Stroke Length

The distance between the lower plunger position and the upper mechanical stop is out of limits (isocratic pump).

During initialization, the isocratic pump monitors the drive current. If the plunger reaches the upper mechanical stop position before expected, the motor current increases as the isocratic pump attempts to drive the plunger beyond the mechanical stop. This current increase causes the error message to be generated.

Probable Causes

- Defective pump drive assembly.

Suggested Actions

- ✓ Exchange the pump drive assembly.

Initialization Failed

The isocratic pump failed to initialize successfully within the maximum time window.

A maximum time is assigned for the complete pump-initialization cycle. If the time is exceeded before initialization is complete, the error message is generated.

Probable Causes

- Blocked active inlet valve.
- Defective pump drive assembly.
- Defective LPM board.

Suggested Actions

- ✓ Exchange the active inlet valve.
- ✓ Exchange the pump drive assembly.
- ✓ Exchange the LPM board.

Wait Timeout

When running certain tests in the diagnostics mode or other special applications, the pump must wait for the plungers to reach a specific position, or must wait for a certain pressure or flow to be reached. Each action or state must be completed within the timeout period, otherwise the error message is generated.

Possible Reasons for a Wait Timeout

- Pressure not reached.
- Pump channel A did not reach the delivery phase.
- Pump channel B did not reach the delivery phase.
- Pump channel A did not reach the take-in phase.
- Pump channel B did not reach the take-in phase.
- Solvent volume not delivered within the specified time.

Probable Causes

- Purge valve still open.
- Leak at fittings, purge valve, active inlet valve, outlet ball valve or plunger seals.
- Flow changed after starting test.
- Defective pump drive assembly.

Suggested Actions

- ✓ Ensure that purge valve is closed.
- ✓ Exchange defective capillaries.
- ✓ Ensure pump components are seated correctly. If there are still signs of a leak, exchange the appropriate seal (purge valve, active inlet valve, outlet ball valve, plunger seal).
- ✓ Ensure correct operating condition for the special application in use.
- ✓ Exchange the defective pump drive assembly.

Pressure Test

Description

The pressure test is a quick, built-in test designed to demonstrate the pressure-tightness of the system. The test should be used when problems with small leaks are suspected, or after maintenance of flow-path components (e.g. pump seals, injection seal) to prove pressure tightness up to 400 bar. The test involves monitoring the pressure profile as the pump runs through a predefined pumping sequence. The resulting pressure profile provides information about the pressure tightness of the system.

The column compartment outlet (or the outlet of the last module before the detector) is blocked with a blank nut, and then the test is run using isopropyl alcohol (IPA), while monitoring the pressure profile (using an integrator on the analog output, or in the plot screen in the ChemStation). The pressure profile is shown in [Figure 8](#).

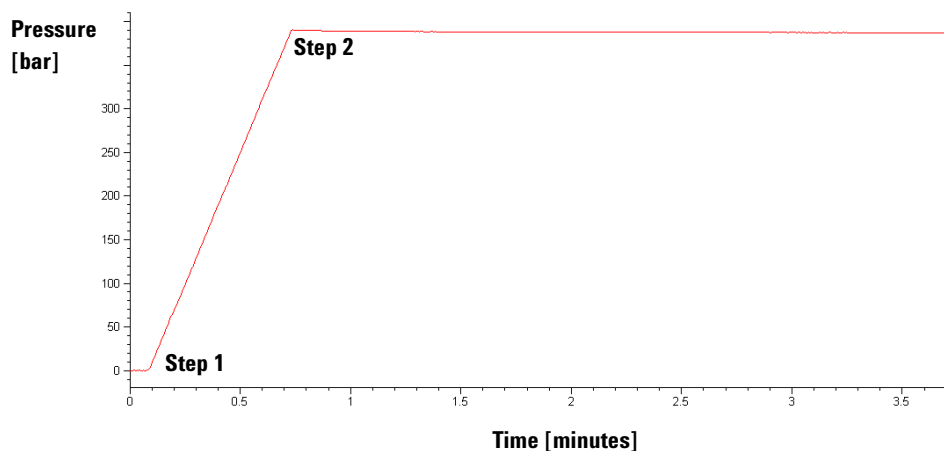


Figure 8 Typical Pressure-Test Pressure Profile with IPA

Step 1

The test begins with the initialization of the pump. After initialization, plunger 1 is at the top of its stroke. Next, the pump begins pumping solvent with a flow rate of 510 µl/min and stroke of 100 µl. The pump continues to pump until a system pressure of 390 bar is reached.

Step 2

When the system pressure reaches 390 bar, the pump switches off. The pressure drop from this point onwards should be no more than 2 bar/minute.

Positioning the blank nut

To test the complete system’s pressure tightness, the blank nut should be positioned at the column compartment outlet (or the outlet of the last module before the detector).

If a specific component is suspected of causing a system leak, place the blank nut immediately before the suspected component, then run the pressure test again. If the test passes, the defective component is located after the blank nut. Confirm the diagnosis by placing the blank nut immediately after the suspected component. The diagnosis is confirmed if the test fails.

Running the Pressure Test

Tools required	¼-inch” wrench
Parts and materials required	Blank nut, 01080-83202
	Isopropanol, 500 ml

Running the test from the ChemStation

- 1 Select the pressure test from the test selection box in the Diagnosis screen.
- 2 Start the test and follow the instructions.

NOTE

Make absolutely sure that all parts of the flow path that are part of the test are very thoroughly flushed with IPA before starting to pressurize the system! Any trace of other solvents or the smallest air bubble inside the flow path definitely will cause the test to fail!

The slope and plateau are evaluated automatically. “[Evaluating the Results](#)” on page 79 describes the evaluation and interpretation of the pressure test results.

Running the test from the Control Module

- 1 Place a bottle of LC-grade isopropyl alcohol in the solvent cabinet and connect it’s solvent tube to the active inlet valve.
- 2 Block column compartment outlet (or the outlet of the last module before the detector) with a blank nut (01080-83202), “[Positioning the blank nut](#)” on page 77
- 3 Open the purge valve. Set flow to 5 ml/min and flush the degasser for about 10 minutes.
- 4 Set flow to 0 ml/min. *Leave the purge valve open.*
- 5 Connect the signal cable to the analog output at the rear of the pump module (only if an integrator is used).
- 6 Press Execute to initialize the pressure test.

Once the test is started, the pump moves the plungers into the start position. When the plungers are in position, the user interface prompts you to close the purge valve, and continue the test.

- 7 Close the purge valve, select *continue* on the control module and press *Enter* to start the test.

The control module displays a graphical representation of the pressure. “[Evaluating the Results](#)” on page 79 describes the evaluation and interpretation of the pressure test results.

- 8 When the test is finished slowly open the purge valve to release the pressure in the system.

Evaluating the Results

The sum of all leaks between the pump and the blank nut will be indicated by a pressure drop of >2 bar/minute at the plateau. Note that small leaks may cause the test to fail, but solvent may not be seen leaking from a module.

NOTE

Please notice the difference between an **error** in the test and a **failure** of the test! An **error** means that during the operation of the test there was an abnormal termination. If a test **failed**, this means that the results of the test were not within the specified limits.

If the pressure test fails:

- Ensure all fittings between the pump and the blank nut are tight. Repeat the pressure test.

NOTE

Often it is only a damaged blank nut itself (poorly shaped from overtightening) that causes a failure of the test. Before investigating on any other possible sources of failure make sure that the blank nut you are using is in good condition and properly tightened!

- If the test fails again, insert the blank nut at the outlet of the previous module in the stack (eg. autosampler, port 6 of the injection valve), and repeat the pressure test. Exclude each module one by one to determine which module is leaking.
- If the pump is determined to be the source of the leak, run the leak test.

Potential Causes of Pressure Test Failure

After isolating and fixing the cause of the leak, repeat the pressure test to confirm the system is pressure tight.

Potential Cause (Pump)	Corrective Action
Purge valve open.	Close the purge valve.
Loose or leaky fitting.	Tighten the fitting or exchange the capillary.
Damaged pump seals or plungers.	Run the leak test to confirm the leak.
Loose purge valve.	Tighten the purge valve nut (14 mm wrench).

3 Troubleshooting and Test Functions

Potential Cause (Autosampler)	Corrective Action
Loose or leaky fitting.	Tighten or exchange the fitting or capillary.
Rotor seal (injection valve).	Exchange the rotor seal.
Damaged metering seal or plunger.	Exchange the metering seal. Check the plunger for scratches. Exchange the plunger if required.
Needle seat.	Exchange the needle seat.

Potential Cause (Column Compartment)	Corrective Action
Loose or leaky fitting.	Tighten or exchange the fitting or capillary.
Rotor seal (column switching valve).	Exchange the rotor seal.

Leak Test

Description

The leak test is a built-in troubleshooting test designed to demonstrate the leak-tightness of the pump. The test should be used when problems with the pump are suspected. The test involves monitoring the pressure profile as the pump runs through a predefined pumping sequence. The resulting pressure profile provides information about the pressure tightness and operation of the pump components.

The pump outlet is blocked with a blank nut, and then the test is run using isopropyl alcohol (IPA), while monitoring the pressure profile (using an integrator on the analog output, or in the plot screen in the Control Module or the ChemStation).

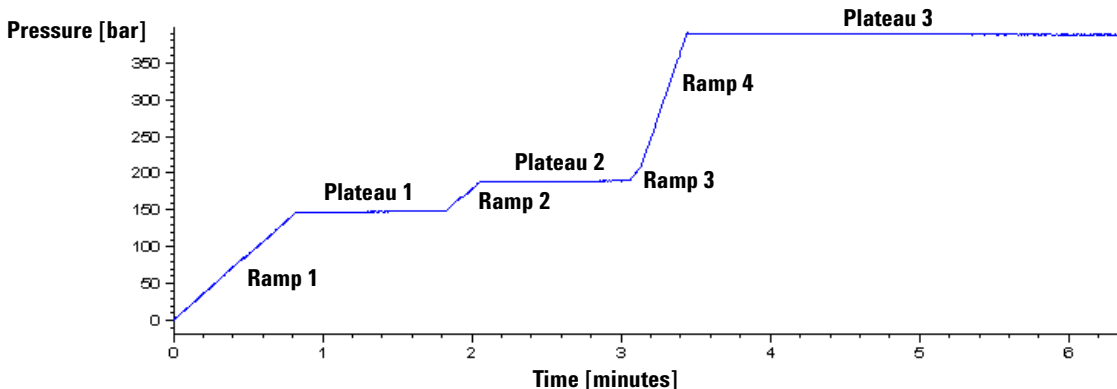


Figure 9 Typical Leak-Test Pressure Profile with IPA

Ramp 1:

After initialization, plunger 2 is at the top of its stroke. The test begins with plunger 1 delivering with a stroke length of 100 μ l and a flow of 153 μ l/min. The plunger sequence during the pressure ramp is 1-2-1-2. The pressure increase during this phase should be linear. Pressure disturbances during this phase indicate larger leaks or defective pump components.

Plateau 1:

plunger 2 continues to pump with a flow rate of 2 μ l/min for approximately one minute. The pressure during the plateau should remain constant or increase slightly. A falling pressure indicates a leak of >2 μ l/min.

Ramp 2:

The flow is changed to 153 μ l/min, and plunger 2 continues to deliver for the rest of its stroke. Then plunger 1 continues to pump to complete the second half of the ramp.

Plateau 2:

The flow is reduced to 2 μ l/min for approximately one minute (plunger 1 still delivering). The pressure during the plateau should remain constant or increase slightly. A falling pressure indicates a leak of >2 μ l/min.

Ramp 3:

The flow increases to 220 μ l/min and the stroke is changed to 100 μ l. Plunger 1 completes its stroke. Next, the flow is changed to 510 μ l/min. The ramp reaches 390 bar with the plunger sequence 2-1-2-1.

Ramp 4:

When the system pressure reaches 390 bar, the flow is reduced to zero, and the pressure stabilizes just below 400 bar.

Plateau 3:

1 min after reaching the maximum pressure, the pressure drop should not exceed 2 bar/min.

Running the Leak Test

Tools required	¼ inch" wrench.
Parts and materials required	Restriction Capillary ,G1313-87305 Blank nut, 01080-83202 Isopropanol, 500 ml

Running the test from the ChemStation

- 1 Select the leak test from the test selection box in the Diagnosis screen.
- 2 Start the test and follow the instructions.

NOTE

Make absolutely sure that all parts of the flow path that are part of the test are very thoroughly flushed with IPA before starting to pressurize the system! Any trace of other solvents or the smallest air bubble inside the flow path definitely will cause the test to fail!

The slopes and plateaus are evaluated automatically. "[Evaluating the Results](#)" on page 79 describes the evaluation and interpretation of the leak test results.

Running the test from the Control Module

- 1 Place a bottle of LC-grade isopropyl alcohol in the solvent cabinet and connect it's solvent tube to the active inlet valve of the pump.
- 2 Open the purge valve.
- 3 Set flow to 5 ml/min and flush the degasser channel for about 10 minutes.
- 4 Turn off pump operation and close the purge valve.
- 5 Connect the restriction capillary (G1313-87305) to pump outlet.

The next steps are necessary to wear in new seals.

- 6 Set flow to 5 ml/min and flush the pump channel for about 3 minutes.
- 7 Set flow to 0 ml/min and replace the restriction capillary with blank nut (01080-83202).
- 8 Open the purge valve.
- 9 Connect the signal cable to the analog output at the rear of the pump module (only if an integrator is used).

3 Troubleshooting and Test Functions

10 Press **Execute** to initialize the leak test.

Once the test is started, the pump moves the plungers into the start position. When the plungers are in position, the user interface prompts you to close the purge valve.

11 Close the purge valve, select *continue* on the control module and press *Enter* to start the test.

The control module displays a graphical representation of the pressure in the plateau windows. "[Evaluating the Results](#)" on page 79 describes the evaluation and interpretation of the leak test results.

12 When the test is finished open the purge valve to release the pressure in the system.

Evaluating the Results

Defective or leaky components in the pump head lead to changes in the leak-test pressure plot. Typical failure modes are described below.

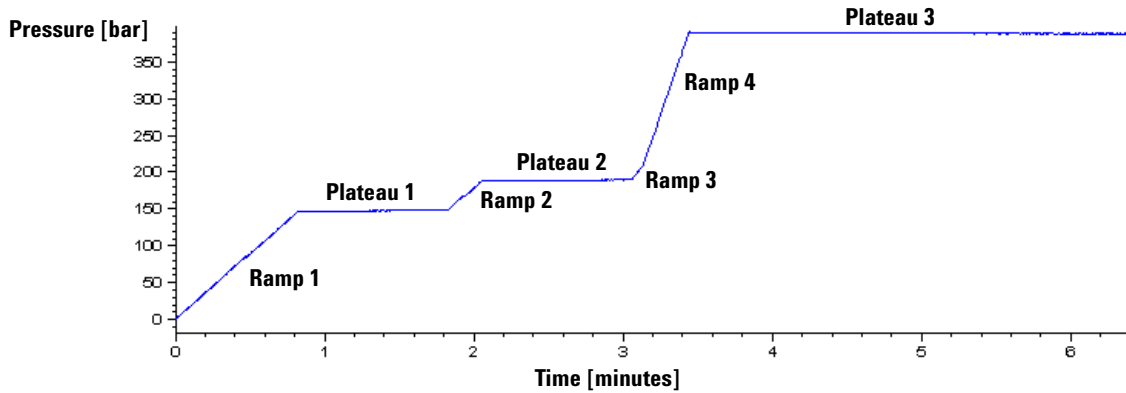


Figure 10 Leak Test Pressure Profile

NOTE

Please notice the difference between an **error** in the test and a **failure** of the test! An **error** means that during the operation of the test there was an abnormal termination. If a test **failed**, this means that the results of the test were not within the specified limits.

NOTE

Often it is only a damaged blank nut itself (poorly shaped from overtightening) that causes a failure of the test. Before investigating on any other possible sources of failure make sure that the blank nut you are using is in good condition and properly tightened!

No Pressure increase at Ramp 1

Potential Cause	Corrective Action
Pump not running.	Check the logbook for error messages.
Purge valve open.	Close the purge valve, and restart the test.
Loose or leaky fittings.	Ensure all fittings are tight, or exchange capillary.

3 Troubleshooting and Test Functions

Wrong solvent-line connections.	Ensure the solvent lines from the degasser are connected correctly.
Contaminated purge valve.	Open and close purge valve to flush out contamination. Exchange the valve if still leaky.
Large leaks (visible) at the pump seals.	Exchange the pump seals.
Large leaks (visible) at active inlet valve, outlet valve, or purge valve.	Ensure the leaky components are installed tightly. Exchange the component if required.

Pressure limit not reached but plateaus horizontal or positive

Potential Cause	Corrective Action
Degasser and pump not flushed sufficiently (air in the pump head).	Purge the degasser and pump thoroughly with isopropanol under pressure (use the restriction capillary).
Wrong solvent.	Install isopropanol. Purge the degasser and pump thoroughly.

All plateaus negative

Potential Cause	Corrective Action
Loose or leaky fittings.	Ensure all fittings are tight, or exchange capillary.
Loose purge valve.	Tighten the purge valve (14mm wrench).
Contaminated purge valve.	Open and close purge valve to flush out contamination. Exchange the valve if still leaky.
Loose pump head screws.	Ensure the pump head screws are tight.
Leaking seals or scratched plungers.	Exchange the pump seals. Check the plungers for scratches. Exchange if scratched.
Leaking outlet valve.	Exchange the outlet valve.
Leaky damper.	Exchange damper.

First plateau positive, second and third plateau negative

Potential Cause	Corrective Action
Air in pump or new seals not yet seated.	Flush pump thoroughly with isopropanol under pressure (use restriction capillary).
Loose active inlet valve.	Tighten the active inlet valve (14mm wrench). Do not overtighten!
Loose pump head screws.	Ensure the pump head screws are tight.
Loose outlet valve.	Ensure the sieve in the outlet valve is installed correctly. Tighten the outlet valve.
Leaking seal or scratched plunger.	Exchange the pump seals. Check the plungers for scratches. Exchange if scratched.
Defective active inlet valve.	Exchange the active inlet valve.

First plateau negative, second plateau positive


Potential Cause	Corrective Action
Leaking outlet valve.	Clean the outlet valve. Ensure the sieve in the outlet valves are installed correctly. Tighten the outlet valve.
Loose pump head screws.	Ensure the pump head screws are tight.
Leaking seals or scratched plungers.	Exchange the pump seals. Check the plunger for scratches. Exchange if scratched.

Ramp 3 does not reach limit

Potential Cause	Corrective Action
Pump stopped due to error.	Check the logbook for error messages.
Large leaks (visible) at the pump seals.	Exchange the pump seals.
Large leaks (visible) at active inlet valve, outlet valve, or purge valve.	Ensure the leaky components are installed tightly. Exchange the component if required.

Third plateau negative (pressure drop > 2 bar/min)

Potential Cause	Corrective Action
Loose or leaky fittings.	Ensure all fittings are tight, or exchange capillary.
Loose purge valve.	Tighten the purge valve (14mm wrench).
Contaminated purge valve.	Open and close purge valve to flush out contamination. Exchange the valve if still leaky.
Loose pump head screws.	Ensure the pump head screws are tight.
Leaking seals or scratched plungers.	Exchange the pump seals. Check the plungers for scratches. Exchange if scratched.
Leaking outlet valve.	Exchange the outlet valve.
Leaky damper.	Exchange damper.

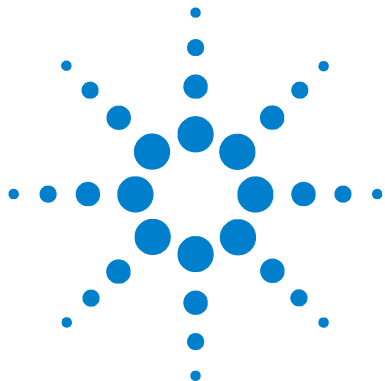

4 Repairing the Pump

Introduction into Repairing the Pump 90

Overview of the Repairing the Pump 92

Simple Repair Procedures 93

Exchanging Internal Parts 117



Introduction into Repairing the Pump

Simple Repairs

The isocratic pump is designed for easy repair. The most frequent repairs such as plunger seal change and purge valve frit change can be done from the front of the isocratic pump with the isocratic pump in place in the system stack. These repairs are described in “[Simple Repair Procedures](#)” on page 93.

WARNING

When opening capillary or tube fittings solvents may leak out. Please observe appropriate safety procedures (for example, goggles, safety gloves and protective clothing) as described in the material handling and safety data sheet supplied by the solvent vendor, especially when toxic or hazardous solvents are used.

Exchanging Internal Parts

Some repairs may require exchange of defective internal parts. Exchange of these parts requires removing the isocratic pump from the stack, removing the covers, and disassembling the isocratic pump. The security lever at the power input socket prevents that the pump cover is taken off when line power is still connected.

WARNING

To prevent personal injury, the power cable must be removed from the isocratic pump before opening the pump cover. Do not connect the power cable to the isocratic pump while the covers are removed.

CAUTION

Electronic boards and components are sensitive to electrostatic discharge (ESD). In order to prevent damage always use an ESD protection (for example, the ESD wrist strap from the accessory kit) when handling electronic boards and components.

Cleaning the Isocratic Pump

The isocratic pump case should be kept clean. Cleaning should be done with a soft cloth slightly dampened with water or a solution of water and a mild detergent. Do not use an excessively damp cloth that liquid can drip into the isocratic pump.

WARNING

Do not let liquid drip into the isocratic pump. It could cause shock hazard and it could damage the isocratic pump.

Using the ESD Strap

Electronic boards are sensitive to electronic discharge (ESD). In order to prevent damage, always use an ESD strap supplied in the standard accessory kit (see "[Accessory Kit G1311-68075](#)" on page 169) when handling electronic boards and components.

- 1 Unwrap the first two folds of the band and wrap the exposed adhesive side firmly around your wrist.
- 2 Unroll the rest of the band and peel the liner from the copper foil at the opposite end.
- 3 Attach the copper foil to a convenient and exposed electrical ground.

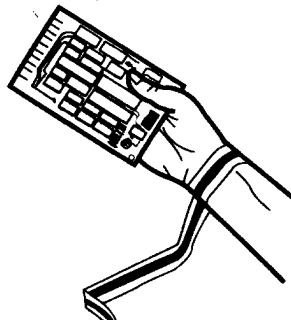


Figure 11 Using the ESD Strap

Overview of the Repairing the Pump

Figure 12 shows the main assemblies of the isocratic pump. The pump head and its parts do require normal maintenance (for example, seal exchange) and can be accessed from the front (simple repairs). Replacing internal parts will require to remove the isocratic pump from its stack and to open the top cover.

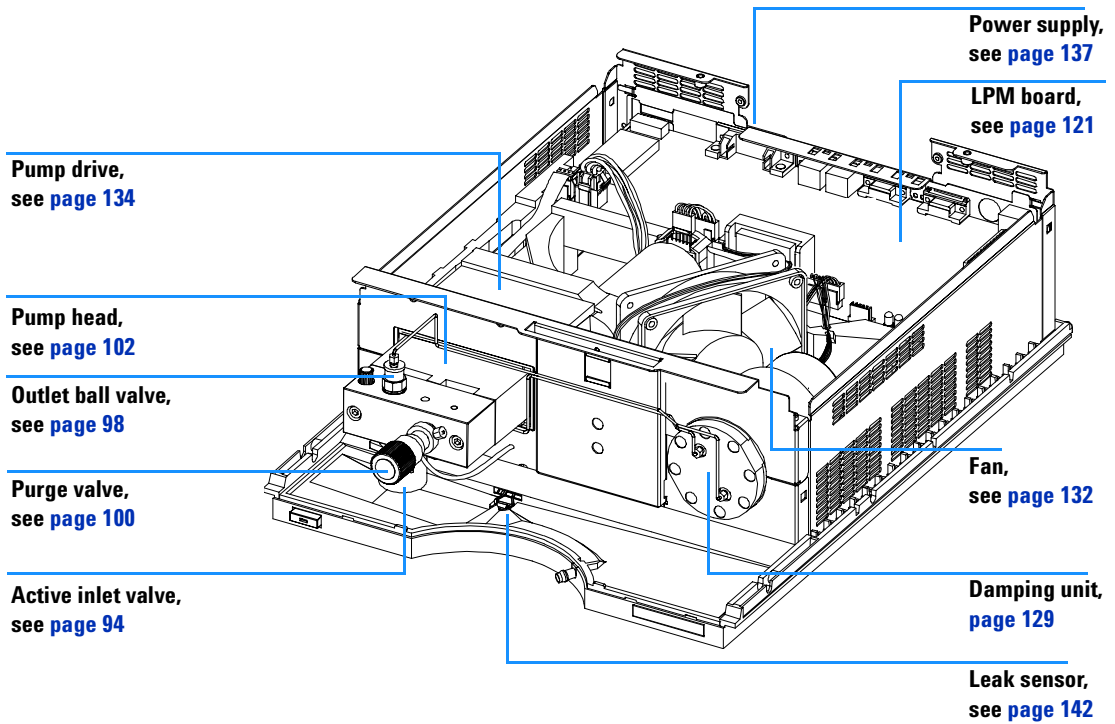


Figure 12 Overview of Repair Procedures

Simple Repair Procedures

The procedures described in this section can be done with the isocratic pump in place in the system stack.

Table 6 Simple Repair Procedures

Procedure	Typical Frequency	Notes
"Exchanging the Active Inlet Valve" on page 94	If internally leaking	Pressure ripple unstable, run leak test for verification
"Exchanging the Outlet Ball Valve" on page 98	If internally leaking	Pressure ripple unstable, run leak test for verification
"Exchanging the Purge Valve Frit or the Purge Valve" on page 100	If internally leaking	Solvent dripping out of waste outlet when valve closed
"Exchanging the Purge Valve Frit or the Purge Valve" on page 100	If the frit shows indication of contamination or blockage	A pressure drop of > 10 bar across the frit (5 ml/min H ₂ O with purge open) indicates blockage
"Exchanging the Pump Seals and Seal Wear-in Procedure" on page 103	If pump performance indicates seal wear	Leaks at lower pump head side, unstable retention times, pressure ripple unstable — run leak test for verification
"Exchanging the Plungers" on page 106	If scratched	Seal life time shorter than normally expected — check plungers while changing the seals
"Installing the Continuous Seal Wash Option" on page 108	If seals show indication of leaks	Leaks at lower pump head side, loss of wash solvent

Exchanging the Active Inlet Valve

When required	If internally leaking (backflow)
Tools required	Wrench 14 mm Pair of Tweezers
Material	Active inlet valve G1312-60010(complete assembly) Valve cartridge 5062-8562
Preparations for this procedure	Switch off isocratic pump at the main power switch

- 1 Remove the front cover
- 2 Unplug the active inlet valve cable from the connector.
- 3 Disconnect the solvent inlet tube at the inlet valve (be aware that solvent may leak out of the tube due to hydrostatic flow).
- 4 Unscrew the adapter from the active inlet valve.
- 5 Using a 14 mm wrench loosen the active inlet valve and remove the valve from pump head.

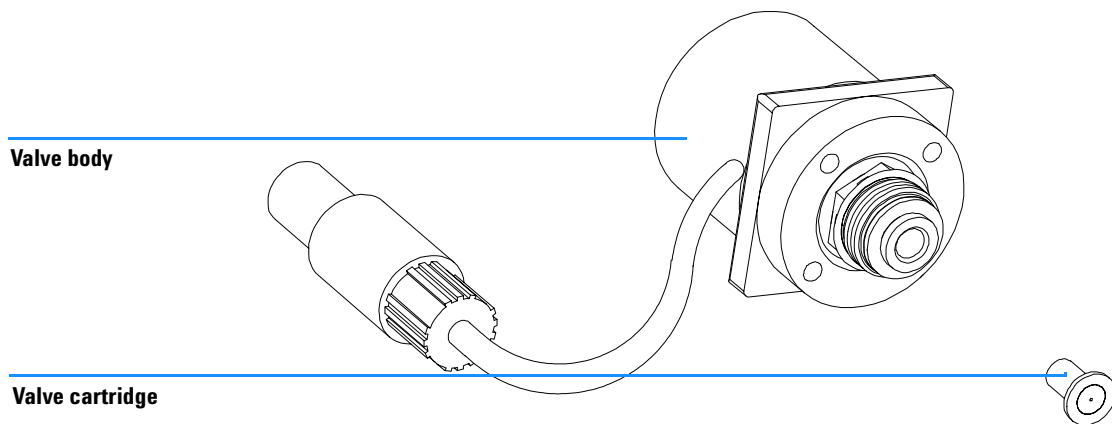


Figure 13 Active Inlet Valve Assembly

- 6 Insert the new valve into the pump head. Using the 14 mm wrench turn the nut until it is hand tight.
- 7 Position the valve so that the solvent inlet tube connection points towards the front.

- 8 Using the 14 mm wrench tighten the nut by turning the valve in its final position (not more than a quarter turn).
- 9 Reconnect the adapter at the active inlet valve.
- 10 Reconnect the solvent inlet tube to the adapter.
- 11 Reconnect the active inlet valve cable to the connector in the Z-panel.
- 12 Reinstall the front cover.

NOTE

After an exchange of the valve it may take several ml of pumping with the solvent used in the current application, before the flow stabilizes at a %-ripple as low as it used to be when the system was still working properly.

Exchanging the Active Inlet Valve Cartridge

When required	If internally leaking (backflow)
Tools required	Wrench 14 mm Pair of Tweezers
Material	Active inlet valve G1312-60010(complete assembly) Valve cartridge 5062-8562
Preparations for this procedure	Switch off isocratic pump at the main power switch

- 1 Remove the front cover
- 2 Unplug the active inlet valve cable from the connector.
- 3 Disconnect the solvent inlet tube at the inlet valve (be aware that solvent may leak out of the tube due to hydrostatic flow).
- 4 Unscrew the adapter from the active inlet valve.
- 5 Using a 14 mm wrench loosen the active inlet valve and remove the valve from pump head.
- 6 Using a pair of tweezers remove the valve cartridge from the actuator assembly.
- 7 Before inserting the new valve cartridge clean the area in the actuator assembly. Flush the cartridge area thoroughly with alcohol.
- 8 Insert a new valve cartridge into the actuator assembly (make sure the valve cartridge is fully inserted into the actuator assembly).
- 9 Insert the valve into the pump head. Using the 14 mm wrench turn the nut until it is hand tight.
- 10 Position the valve so that the solvent inlet tube connection points towards the front.
- 11 Using the 14 mm wrench tighten the nut by turning the valve in its final position (not more than a quarter turn).
- 12 Reconnect the adapter at the active inlet valve.
- 13 Reconnect the solvent inlet tube to the adapter. Reconnect the active inlet valve cable to the connector in the Z-panel.
- 14 Reinstall the front cover.

NOTE

After an exchange of the valve cartridge it may take several ml of pumping with the solvent used in the current application, before the flow stabilizes at a %-ripple as low as it used to be when the system was still working properly.

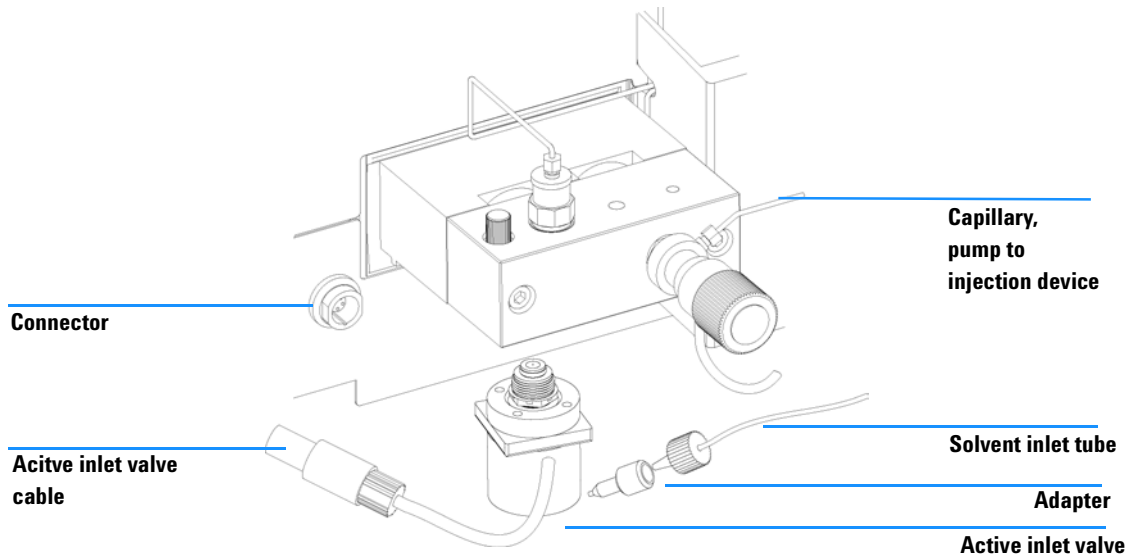


Figure 14 Exchanging the Active Inlet Valve

Exchanging the Outlet Ball Valve

When required	If internally leaking
Tools required	Wrench 1/4 inch Wrench 14 mm
Parts required	Outlet ball valve G1311-60012
Preparations for this procedure	Switch off isocratic pump at the main power switch Remove the front cover

NOTE

Before exchanging the outlet ball valve you can try to clean it in a sonic bath for 5 – 10 minutes. Place the valve in an upright position in a small beaker with alcohol.

- 1 Using a 1/4 inch wrench disconnect the valve capillary from the outlet ball valve.
- 2 Using the 14 mm wrench loosen the valve and remove it from the pump body.
- 3 Check that the new valve is assembled correctly and that the gold seal is present (if the gold seal is deformed, it should be replaced).

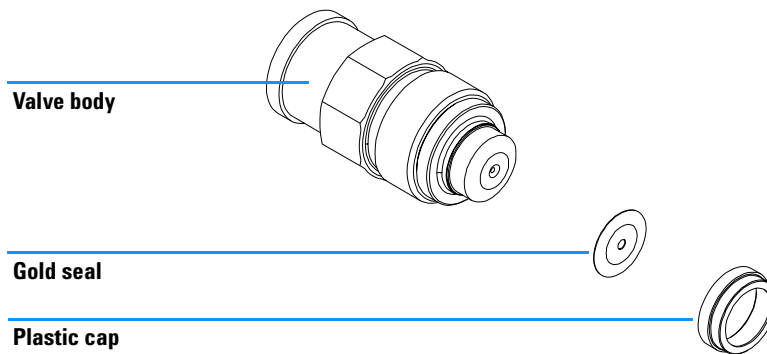


Figure 15 Outlet Ball Valve Parts

- 4 Reinstall the outlet ball valve and tighten the valve.
- 5 Reconnect the valve capillary.

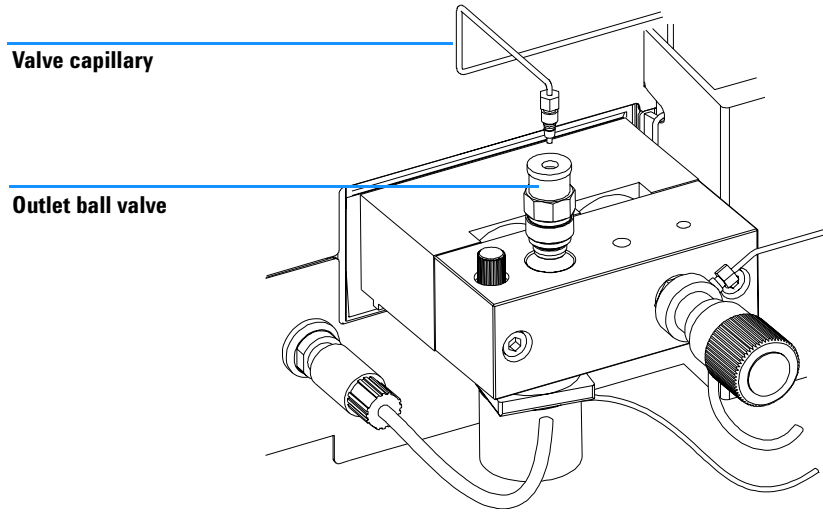


Figure 16 Exchanging the Outlet Ball Valve

Exchanging the Purge Valve Frit or the Purge Valve

When required	Frit – when plunger seals are exchanged or when contaminated or blocked (pressure drop of > 10 bar across the frit at a flow rate of 5 ml/min of H ₂ O with purge valve opened)
Tools required	Purge valve – if internally leaking Wrench 1/4 inch Wrench 14 mm Pair of tweezers or toothpick
Parts required	PTFE frit (pack of 5) 01018-22707 Purge valve G1311-60009
Preparations for this procedure	Switch off isocratic pump at the main power switch Remove the front cover

- 1 Using a 1/4 inch wrench disconnect the pump outlet capillary at the purge valve.
- 2 Disconnect the waste tube. Beware of leaking solvents due to hydrostatic pressure.
- 3 Using the 14 mm wrench unscrew the purge valve and remove it.
- 4 Remove the plastic cap with the gold seal from the purge valve.
- 5 Using a pair of tweezers or a toothpick remove the frit.

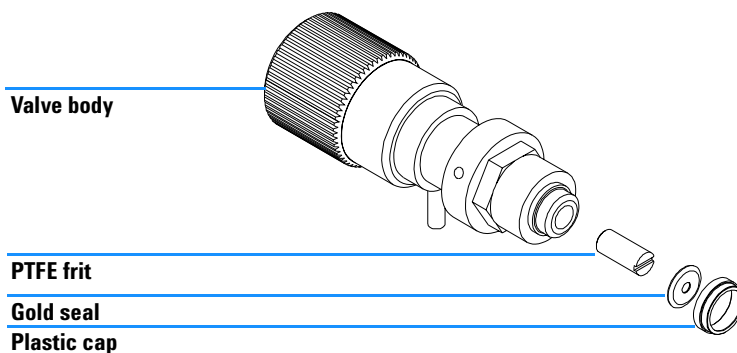


Figure 17 Purge Valve Parts

- 6 Place a new frit into the purge valve with the orientation of the frit as shown above.
- 7 Reinstall the cap with the gold seal.

NOTE

Before reinstallation always check the gold seal. A deformed seal should be exchanged.

8 Insert the purge valve into the pump head and locate the pump outlet capillary and the waste tube as shown in [Figure 18](#).

9 Tighten the purge valve and reconnect outlet capillary and waste tubing.

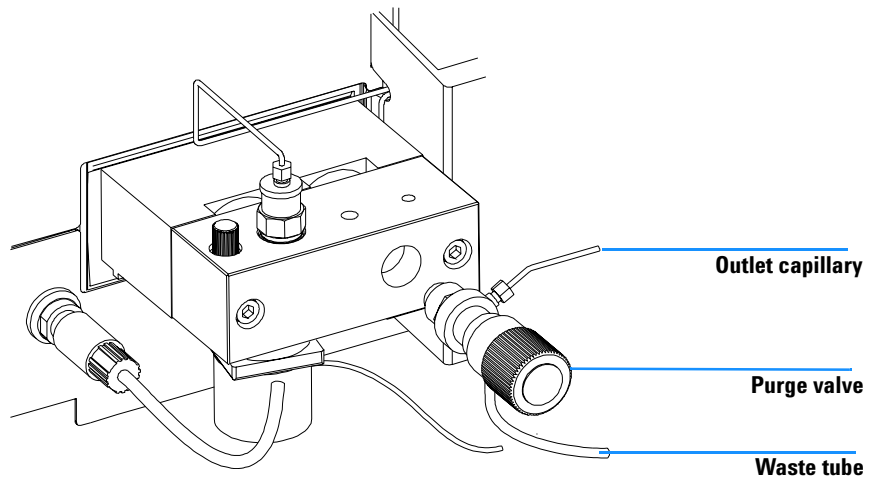


Figure 18 Exchanging the Purge Valve

Removing the Pump Head Assembly


WARNING

Never start the pump when the pump head is removed. This may damage the pump drive.

When required	Exchanging the seals Exchanging the plungers
Tools required	Exchanging seals of the seal wash option Wrench 1/4 inch 4-mm hexagonal key

Preparations for this procedure Switch off isocratic pump at the main power switch

- 1 Remove the front cover.
- 2 Disconnect the Active Inlet Valve cable.
- 3 Using a 1/4 inch wrench remove the outlet capillary.

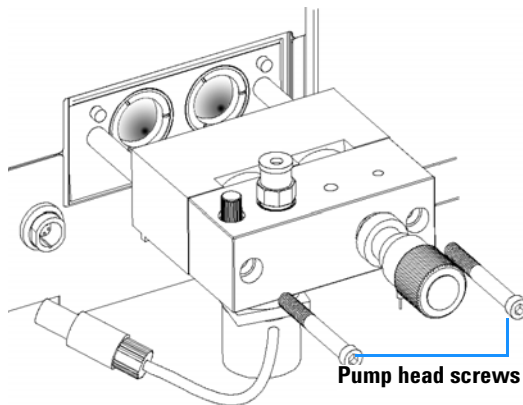


- 4 Disconnect the capillary from the Outlet Ball Valve.
- 5 Remove the waste tubing and disconnect the Active Inlet Valve tubing.
- 6 Remove the capillary at the bottom of the Pumphead.
- 7 Using a 4 mm hexagonal key, stepwise loosen the two Pumphead screws and remove the Pumphead from the Pump Drive.


Exchanging the Pump Seals and Seal Wear-in Procedure

When required	Seal leaking, if indicated by the results of the leak test.
Tools required	Wrench 1/4 inch 4-mm hexagonal key
Parts required	Seals (pack of 2) 5063-6589 (standard) <u>or</u> 0905-1420 (for normal phase applications)
Preparations for this procedure	For the seal wear-in procedure: Adapter AIV to inlet tube (0100-1847) Restriction capillary (5022-2159) Switch off isocratic pump at the main power switch Remove the front cover "Removing the Pump Head Assembly" on page 102

1 Place the pump head on a flat surface. Loosen the lock screw (two revolutions) and while holding the lower half of the assembly carefully pull the pump head away from the plunger housing.

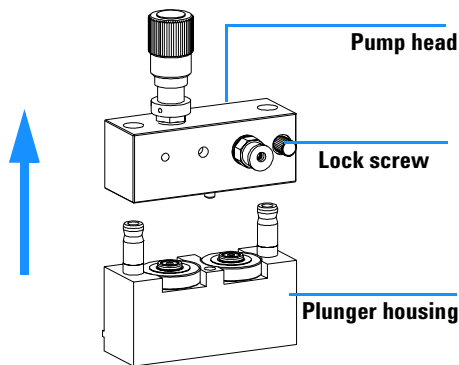


2 Remove the support rings from the plunger housing and lift the housing away from the plungers.

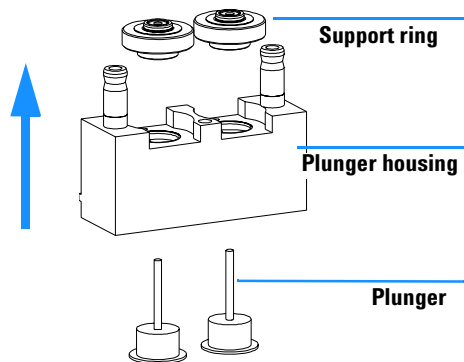


4 Repairing the Pump


3 Using one of the plungers carefully remove the seal from the pump head (be careful not to break the plunger). Remove wear retainers, if still present.

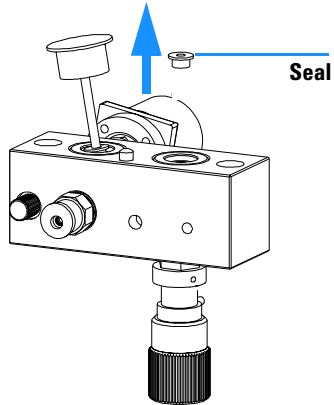

4 Insert new seals into the pump head.

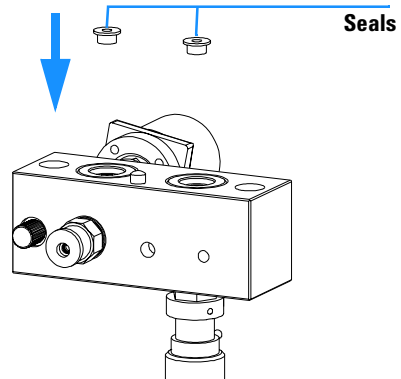

5 Reassemble the Pumphead assembly.

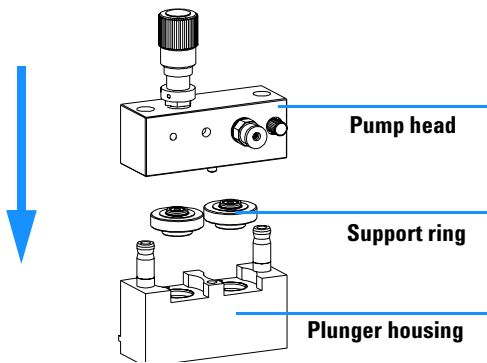

6

Seal Wear-in Procedure

NOTE

This procedure is required for standard seals only (5063-6589), but it will definitely damage the normal phase application seals (0905-1420).

- 1** Place a bottle with 100 ml of Isopropanol in the solvent cabinet and place a tubing (including bottle head assembly) in the bottle.
- 2** Screw the adapter (0100-1847) to the AIV and connect the inlet tube from the bottle head directly to it.
- 3** Connect the restriction capillary (5022-2159) to the purge valve. Insert its other end into a waste container.
- 4** Open the purge valve and purge the system for 5 minutes with isopropanol at a flow rate of 2 ml/min.
- 5** Close the purge valve, set the flow to a rate adequate to achieve a pressure of 350 bar. Pump 15 minutes at this pressure to wear in the seals. The pressure can be monitored at your analog output signal, with the handheld controller, Chemstation or any other controlling device connected to your pump.
- 6** Turn OFF the pump, slowly open the purge valve to release the pressure from the system, disconnect the restriction capillary and reinstall the bottle with the solvent for your application.
- 7** Rinse your system with the solvent used for your next application.

4 Repairing the Pump

Exchanging the Plungers


When required
Tools required

When scratched
Wrench 1/4 inch
4-mm hexagonal key


Parts required
Preparations for this procedure

Plunger 5063-6586
Switch off isocratic pump at the main power switch
Remove the front cover
["Removing the Pump Head Assembly"](#) on page 102


1 Disassemble the Pumphead assembly.

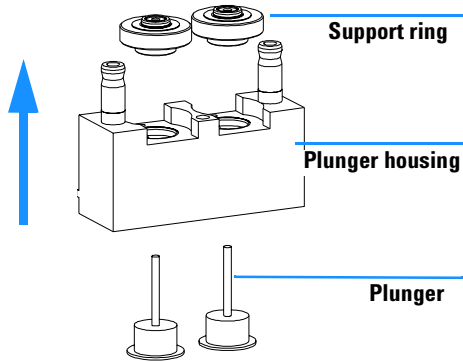

2 Check the plunger surface and remove any deposits or layers. Cleaning can be done with alcohol or tooth paste. Replace plunger if scratched.

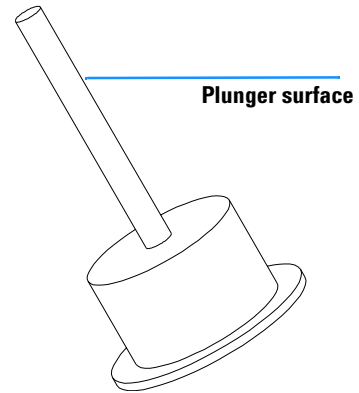

3 Reassemble the Pumthead assembly.

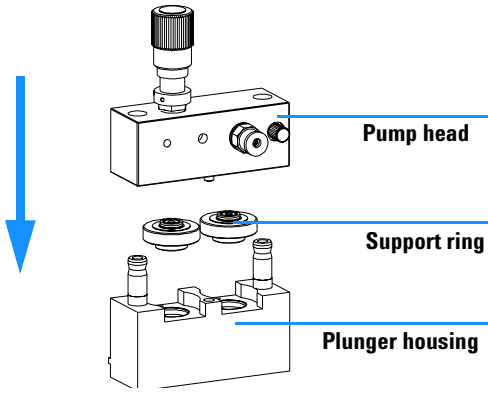


4 Repairing the Pump


Installing the Continuous Seal Wash Option

When required	When installing seal wash option
Tools required	4-mm hexagonal key
Parts required	Seal wash kit 01018-68722
Preparations for this procedure	Switch off isocratic pump at the main power switch Remove the front cover


1 Disconnect all capillaries and tubes from the pump head and disconnect the active inlet valve cable.

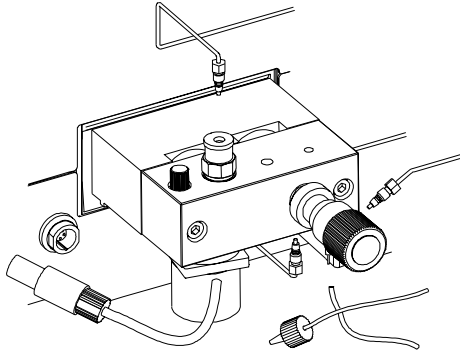


2 Using a 4-mm hexagonal key stepwise loosen and remove the two pump head screws and remove the pump head from the pump drive.

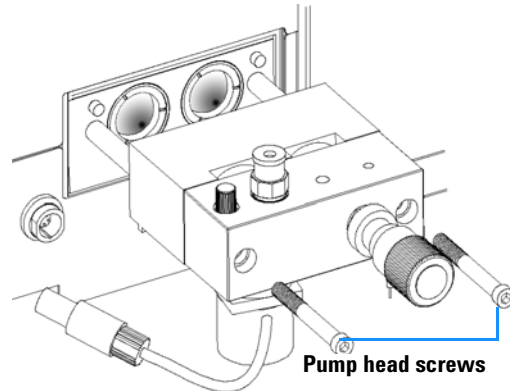


3 Place the pump head on a flat surface. Loosen the lock screw (two revolutions) and while holding the lower half of the assembly carefully pull the pump head away from the plunger housing.

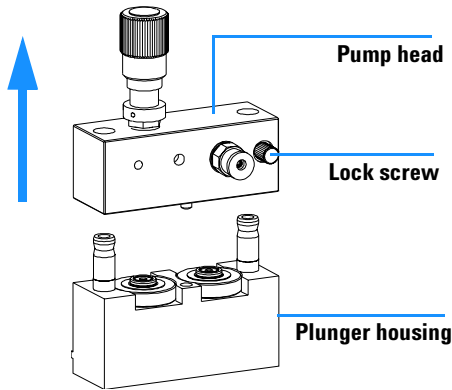


4 Remove the support rings from the plunger housing and lift the housing away from the plungers.

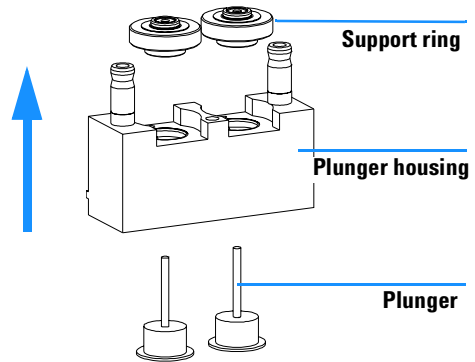

5 Install the support ring assembly from the seal wash option kit into the plunger housing.

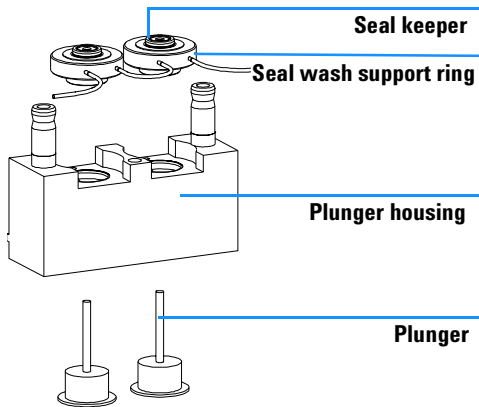


6 Place the support rings on the plunger housing (plungers not installed) and snap the pump head and plunger housing together.

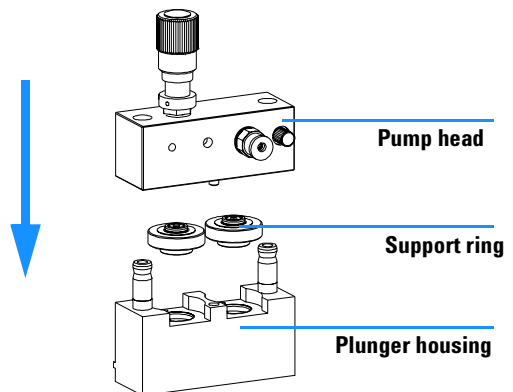


4 Repairing the Pump


7 Insert the plungers and carefully press them into the seal.

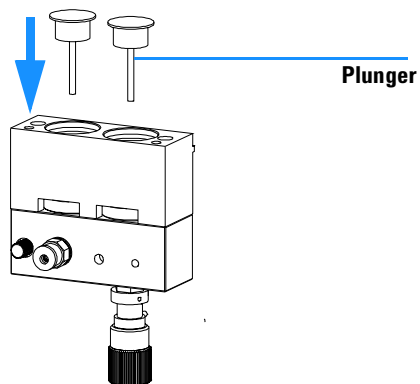


8 Tighten the lock screw.

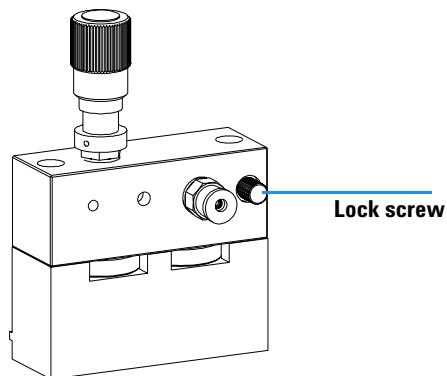

9 Slide the pump head assembly onto the metering drive. Apply a small amount of pump head grease to the pumphead screws and the balls of the spindle drive. Tighten the pumphead screws stepwise with increasing torque.

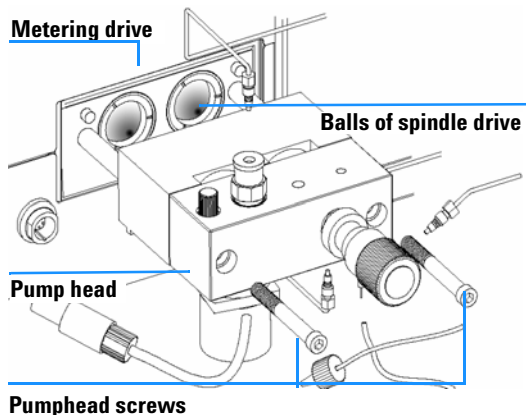

10 Reconnect all capillaries, tubes and the active inlet valve cable to its connector.

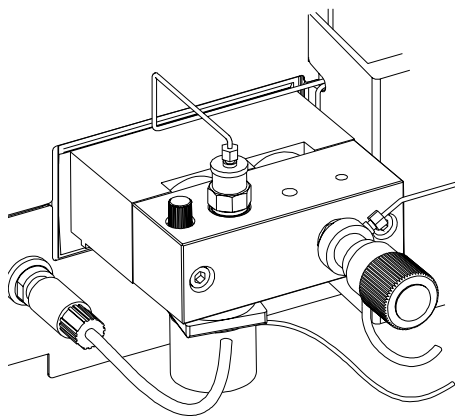

8 Route the wash inlet tube into a bottle filled with a mixture of distilled water and isopropanol (90/10) and place the bottle above the pump (hydrostatic pressure) in the solvent cabinet.

9 Route the outlet of the wash tube into a waste container.

10 The flow rate should be set to approximately 20 drops/minute. Use the velocity regulator attached to the wash tube to regulate the flow rate.

NOTE

The seals should never run dry. Running dry will significantly reduce the lifetime of the seals.

4 Repairing the Pump

Exchanging the Wash Seals

When required

Tools required

Parts required

Preparations for this procedure

When maintaining seal wash option

4-mm hexagonal key


Wash seal 0905-1175

Gasket, seal wash (pack of 6) 5062-2484


Switch off isocratic pump at the main power switch

Remove the front cover


1 Disconnect all capillaries and tubes from the pump head and disconnect the active inlet valve cable.

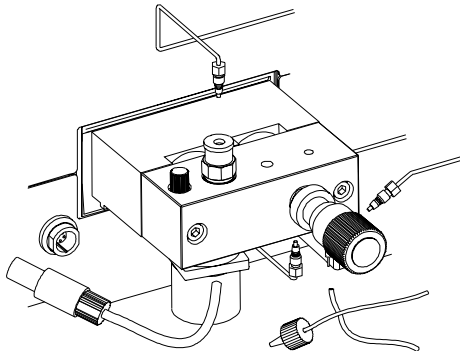


2 Using a 4-mm hexagonal key stepwise loosen and remove the two pump head screws and remove the pump head from the pump drive.

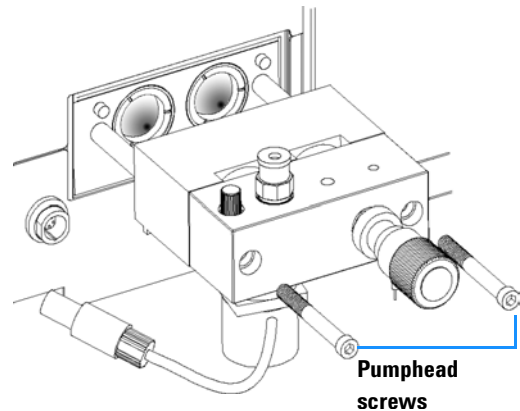


3 Remove the seal keeper and the seal wash support rings from the plunger housing. Remove the seal keeper from the support ring assembly.

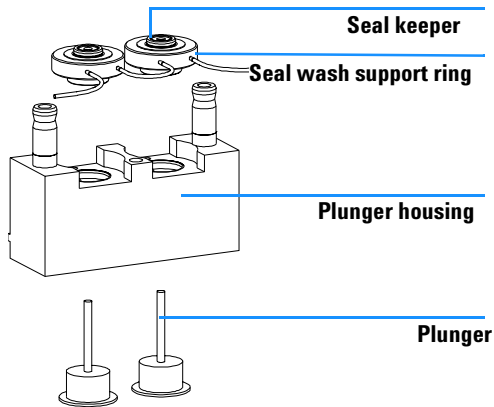


4 Using the blade of a flat-blade screwdriver remove the seal wash gasket and the secondary seal from the support ring.

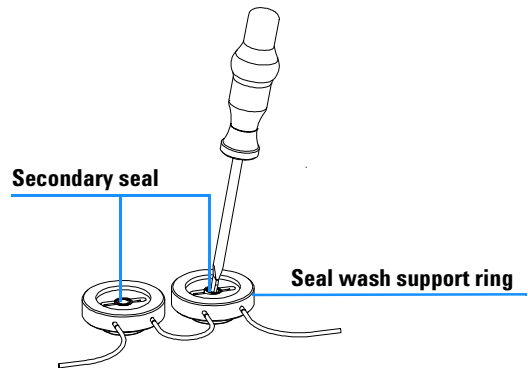

5 Using the insert tool press the secondary seal (spring pointing upwards) into the recess of the support ring. Place a seal wash gasket in the recess of the support ring.

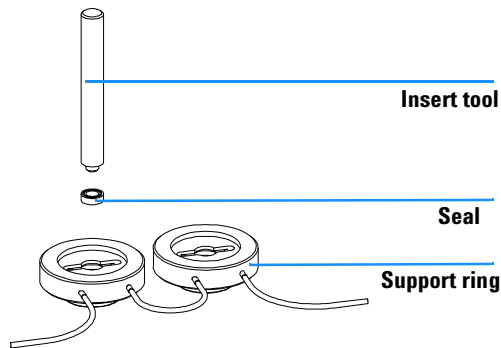


6 Place the support rings on the plunger housing (plungers not installed) and snap the pump head and plunger housing together.

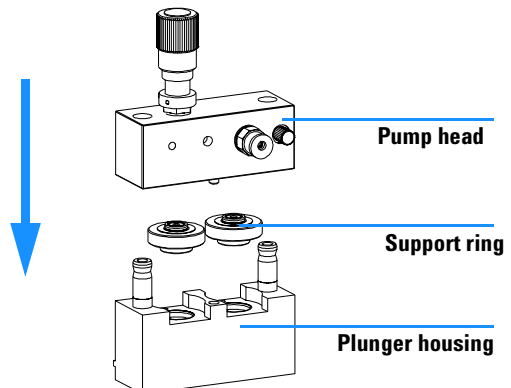


4 Repairing the Pump


7 Insert the plungers and carefully press them into the seal.

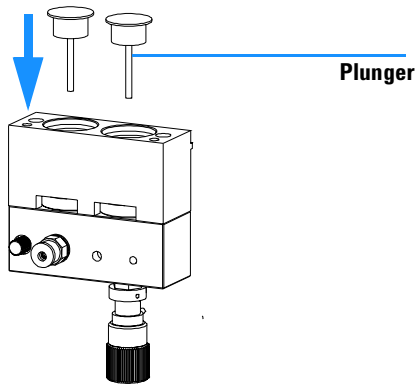


8 Tighten the lock screw.

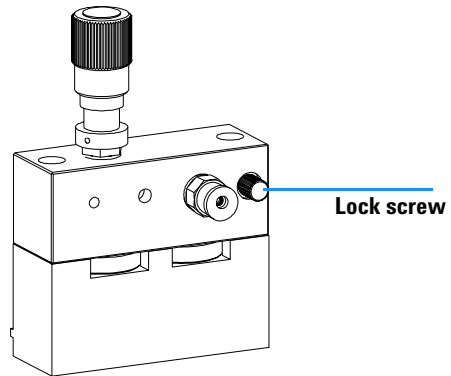

9 Slide the pump head assembly onto the metering drive. Apply a small amount of pump head grease to the pumphead screws and the balls of the spindle drive. Tighten the pumphead screws stepwise with increasing torque.

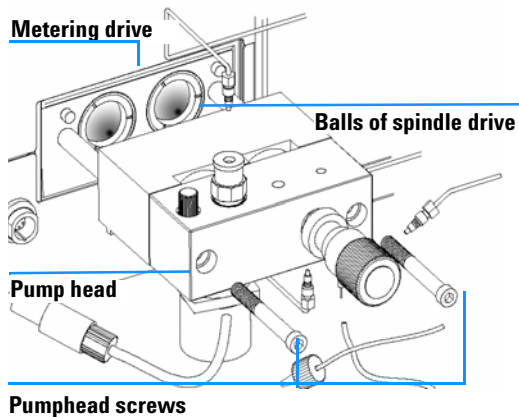


10 Reconnect all capillaries, tubes and the active inlet valve cable to its connector.

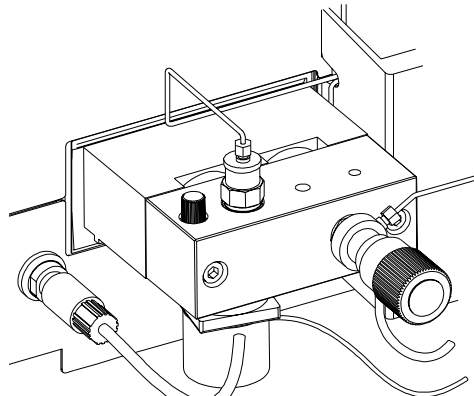

Reinstalling the Pump Head Assembly

When required	When reassembling the pump
Tools required	4-mm hexagonal key
Parts required	Pump head grease (79846-65501)

- 1 Apply a small amount of grease on the back of the pistons.
- 2 Slide the Pumphead Assembly onto the Pumpdrive.
- 3 Using a 4 mm hexagonal key tighten the Pumphead screws stepwise with increasing torque.

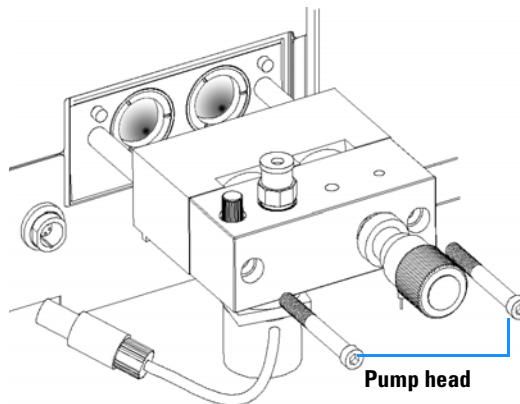

- 4 Reconnect the capillaries, tubing and the Active Inlet Valve cable to the connector.
- 5 Reinstall the front cover.

Exchanging the optional Interface Board

CAUTION

The interface board is sensitive to electrostatic discharge. Always use the ESD kit when handling electronic boards.

When required	Board defective
Parts required	BCD (Interface) board (G1351-68701), see "Optional Interface Boards" on page 208

- 1 Switch off the isocratic pump at the main power switch, unplug the pump from line power.
- 2 Disconnect cables from the interface board connectors.
- 3 Loosen the screws. Slide out the interface board from the isocratic pump.
- 4 Install the new interface board. Secure screws.
- 5 Reconnect the cables to the board connector.

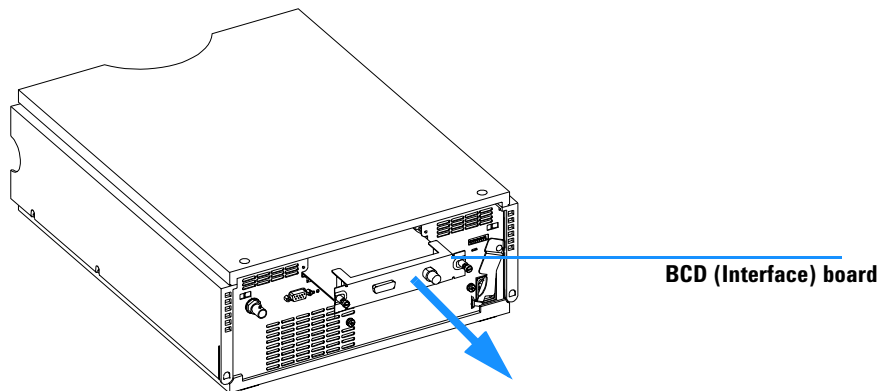


Figure 19 Exchanging the Interface Board

Exchanging Internal Parts

WARNING

The following procedures require opening the main cover of the isocratic pump. Always ensure the isocratic pump is disconnected from the line power when the main cover is removed. The security lever at the power input socket prevents that the pump cover is taken off when line power is still connected.

WARNING

To disconnect the isocratic pump from line, unplug the power cord. The power supply still uses some power, even if the switch on the front panel is turned off.

WARNING

When opening capillary or tube fittings solvents may leak out. Please observe appropriate safety procedures (for example, goggles, safety gloves and protective clothing) as described in the material handling and safety data sheet supplied by the solvent vendor, especially when toxic or hazardous solvents are used.

NOTE

The electronics of the isocratic pump will not allow operation when the top cover and the top foam are removed. A safety light switch on the main board will inhibit the operation of the isocratic pump. Always operate the isocratic pump with the top foam and top covers in place.

CAUTION

Internal components may be sensitive to electrostatic discharge (ESD). Always use an ESD kit when handling internal parts.

The procedures in this section describe how to exchange internal parts. You must remove the isocratic pump from the stack in order to open the main cover.

4 Repairing the Pump

Removing the Top Cover and Foam

Tools required

Screwdriver Pozidriv #1

Preparations for this procedure

Switch off isocratic pump at the main power switch.


Disconnect the solvent inlet and outlet tubes from the pump.

Beware of leaking solvents due to hydrostatic flow.


Remove the solvent cabinet from the isocratic pump.

Remove leak funnel with the waste tube from the top cover of the isocratic pump.


1 Remove the front cover by pressing the both clip fasteners on both sides of the cover.

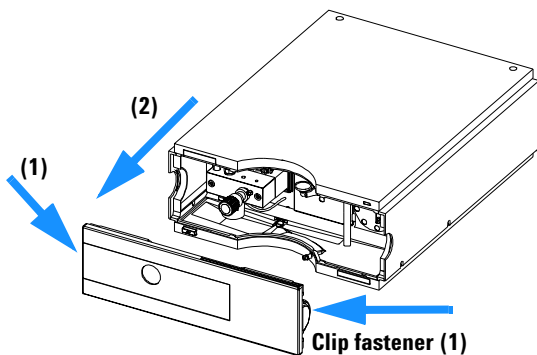


2 Unplug the power cord and move the lever towards the power socket.

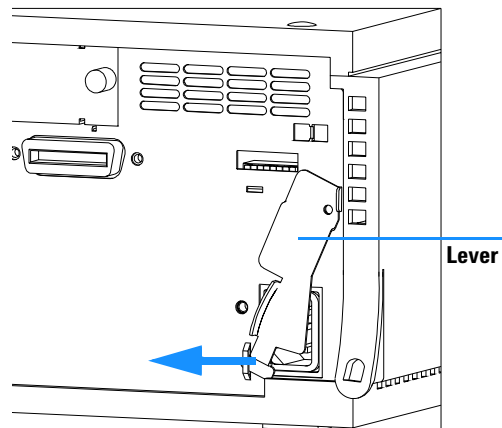


3 Lift the clips on both sides of the top cover (1). Remove the top cover (2).

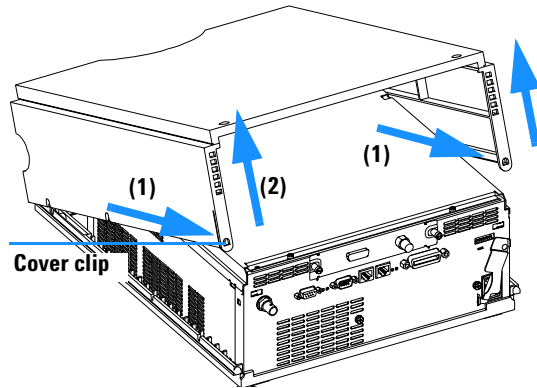


4 Unscrew the screws on the top plate and remove the plate by lifting its back first and then sliding to the front.

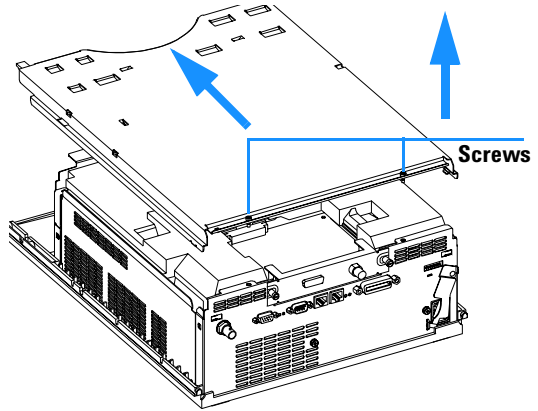

5 If an optional interface board is installed, remove it from the pump slot.

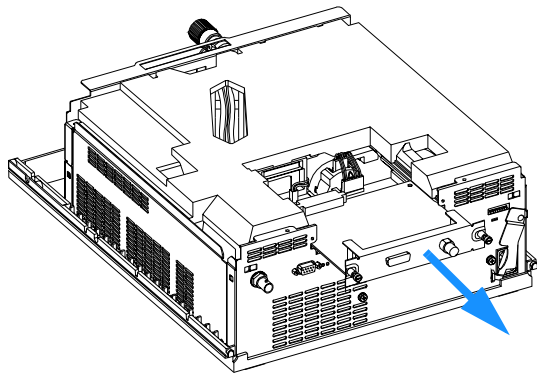

6 Remove the top foam.

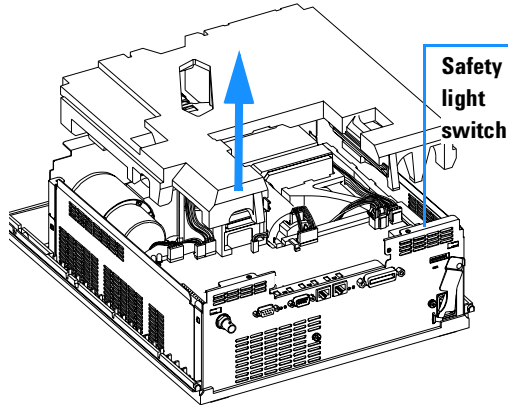


4 Repairing the Pump

Do not connect a power plug to the isocratic pump after removing the top covers.

A safety light switch on the main board will prevent operation when the covers are removed.

The next figure shows the position of the safety light switch on the board.

7 Note the position of the safety light switch on the main board

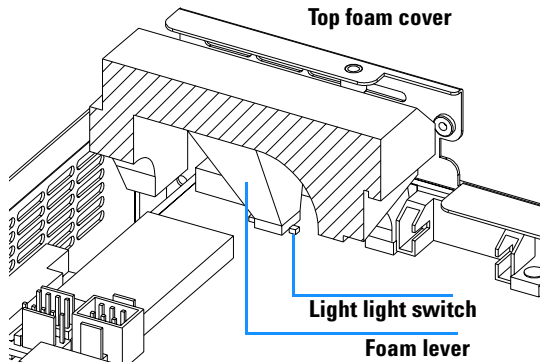

Exchanging the Low Pressure Pump Main Board (LPM Board)

When required	Board defective
Tools required	Wrench 14 mm Wrench 7 mm Wrench 5 mm
Parts required	LPM Board, G1311-66520, exchange part number G1311-69520

- 1 Turn off the pump, disconnect all cables and remove the pump from the stack.
- 2 Remove the top cover and foam (see [“Removing the Top Cover and Foam”](#) on page 118).
- 3 Disconnect all connectors from the main board.

NOTE

When removing connectors, counterhold on connector J3 with one hand.

4 Repairing the Pump

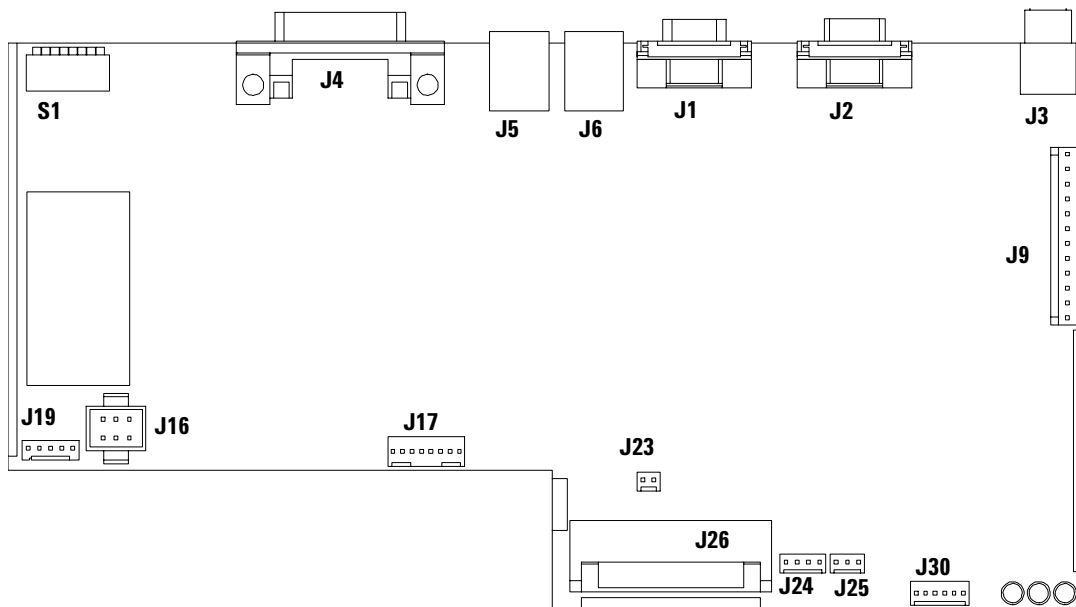


Figure 20 LPM Board Connectors

Connector	Description	Connector	Description
J1	RS232	J17	Encoder
J2	Remote	J19	AIV
J3	Analog Pressure signal	J23	Leak sensor
J4	GPIB	J24	Damper
J5/6	CAN connector	J25	Fan
J9	Power supply	J26	Interface board
J16	Motor	J30	Not used

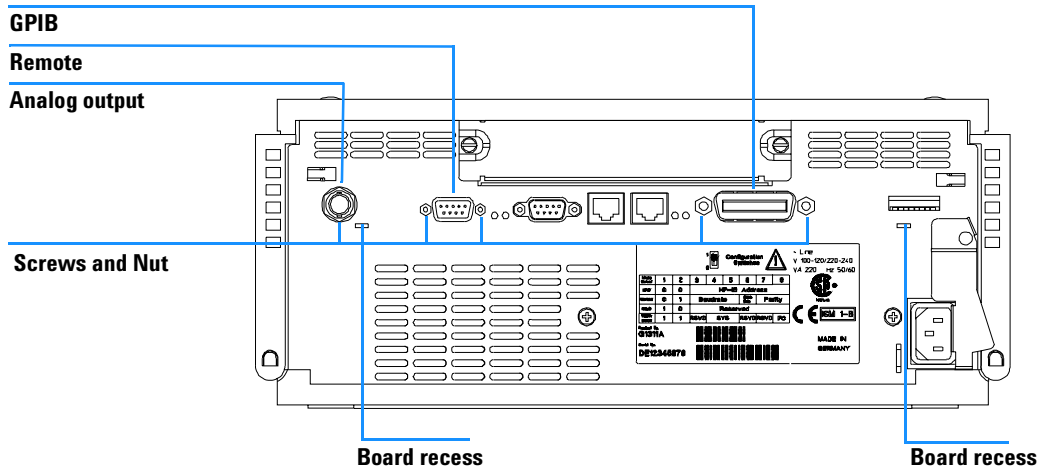


Figure 21 Removing the Screws at the Back Plane.

- 4 Remove the connector screws from the GPIB, Remote and the analog pressure output connector.
- 5 Remove the board. Place the board on an ESD kit.

WARNING

The RFI spring plate sitting on the board connectors is very sharp! Be careful, not to cut yourself, when removing it from the old board and sliding it onto the new board.

- 6 In most cases the RFI spring plate (Radio Frequency Interference spring plate, prevents radio emissions from the instrument to ambient) remains on the interface connectors of the board. Carefully remove the spring plate from the old board and slide it onto the new board before installing the board in the pump (the RFI spring plate is NOT part of an exchange board).

NOTE

If you have to exchange other parts also, continue with that work, first.

- 7 On the new board check the switch setting of address switch S1, see "Setting the 8-bit Configuration Switch" on page 216.

NOTE

An incorrect switch setting (e.g., TEST/BOOT) may cause the pump to turn into a basic mode (yellow or red flashing status light). In such a case turn off the pump, re-set the address switches, and turn on the pump again.

- 8 Install the new board and reconnect the connectors. Make sure that the board is fitted correctly in the board recess holes at the rear panel.
- 9 Refit the connector screws, and reconnect all connectors. Ensure the connectors are seated securely.
- 10 Replace foam and top covers, see [“Replacing the Top Cover and Foam”](#) on page 146.
- 11 Reinstall the pump in the stack. Reconnect all cables. Turn on the isocratic pump. If pump status indicator turns red continue with the section [“Entering the Type Command”](#) on page 124, otherwise continue with [“Entering the Serial Number”](#) on page 126.

Entering the Type Command

NOTE

The main board is physically identical for the isocratic and the quaternary pump. After the installation of a new mainboard the *TYPE* (isocratic or quaternary) of the module is normally automatically detected. The specific *TYPE* tells the pump how to configure itself during turn on. In some cases, especially when a defective mainboard is replaced with an older version of mainboard, the automatic *TYPE* detection does not work. When the *TYPE* of the exchange main board does not match the pump, a pump configuration error will occur during pump turn on. This will cause the pump status indicator to be red. In this case the *TYPE* of the module has to be entered using the procedure described in the following sections.

You must change the *TYPE* of the replacement main board to agree with the isocratic pump (G1310A). The *TYPE* can be entered using either the control module or the ChemStation, see [“Entering the Type Command using the Control Module”](#) on page 124 or [“Entering the Type Command using the ChemStation”](#) on page 125.

Entering the Type Command using the Control Module

- 1 Connect the control module to the pump.
- 2 From *Views* (press F5) select the *System* screen, then press *Tests* (F3).

- 3 Using the up/down arrows, make sure that the isocratic pump is highlighted and press *Enter*. The Tests screen for the isocratic pump should now be displayed.
- 4 While in the *Tests* screen, press m.m (m dot m). From the box now displayed, select the *Command* line, and press *Enter*.
- 5 Into the box labeled *Instr*, enter the command TYPE G1310A.
- 6 Letters and numbers are created using the up and down arrows. There must be a blank space between the word TYPE and the letter G.

NOTE

It is important to enter the TYPE command correctly. An incorrect type command may cause the module to turn on in it's resident mode. In such a case, re-enter the TYPE command correctly.

- 7 When the command is entered, press *Enter* to highlight the complete command.
- 8 Press the *Execute* (F8) key. Below the box, a reply line should then say: Reply RA 0000 TYPE "G1310A" .
- 9 Turn off the module, then turn it on again. Turn on should be normal. In the *Records* screen, the product# column should indicate the isocratic pump. If a ChemStation is also connected, re-boot it now.

Entering the Type Command using the ChemStation

The TYPE is entered by typing a specific command into the command line at the bottom of the main user interface screen.

- 1 To enter the TYPE for a specific module, type the following command into the command line:

```
print sendmodule$(lpmp, "TYPE G1310A")
```

NOTE

It is important to enter the TYPE command correctly. An incorrect type command may cause the module to turn on in it's resident mode. In such a case, re-enter the TYPE command correctly.

- 2 The reply line will respond with RA 0000 Type "G1310A".

4 Repairing the Pump

- 3 Turn the isocratic pump off, then on again. Then, re-boot the ChemStation. Boot up and subsequent control of the system should be normal.
- 4 The TYPE of a module can also be identified by typing the following command into the command line:

```
print sendmodule$ (lpmp, "TYPE?")
```

The reply line will give the module TYPE.

Entering the Serial Number

Entering the Serial Number using the Control Module

- 1 Connect the control module to the isocratic pump. Turn on the pump.
- 2 In the control module, press *Views (F5)* and select the *system* screen, then press *Records (F4)*. Using the up/down arrows, make sure that the isocratic pump is highlighted.
- 3 Press *FW Update (F5)*. Now, press the *m* key. This will display a box which says *Update Enter Serial#*.
- 4 Press *Enter*. This will display the box labeled *Serial#*.
- 5 Letters and numbers are created using the up and down arrows. Into the box labeled *Serial#*, enter the 10-character serial number for the isocratic pump. When the 10-character serial number is entered, press *Enter* to highlight the complete serial number. Then, press *Done (F6)*.

NOTE

For firmware revisions below A02.00 it is very important never to press *Done* if the *Serial#* box is blank. In this case, the module can no longer be recognized by either the control module or the ChemStation. The main board must then be replaced.

- 6 Turn the isocratic pump off, then on again. The *Records* screen should display the correct serial number.
- 7 If a ChemStation is also connected, re-boot the ChemStation now as well.

Entering the Serial Number using the ChemStation

Module serial numbers are entered by typing specific commands into the command line at the bottom of the main user interface screen.

- 1 To enter a module serial number, type the following command into the command line:

```
print sendmodule$(lpmp, "ser YYYYYYYYYY")
```

Where: YYYYYYYYYY is the 10-character serial number of the isocratic pump

NOTE

The first two characters are letters, which should be capitalized.

The reply line will respond with RA 0000 SER followed by the module serial number you just entered.

- 2 Turn off the isocratic pump, then on again. Then, re-boot the ChemStation. If the serial number you have just entered is different than the original module serial number, you will be given the opportunity to edit the configure 1100 access screen during the re-boot of the ChemStation.
- 3 After boot-up, the serial number you have just entered can be seen under the *Instrument menu* of the main user interface screen. The serial number of the isocratic pump can also be seen by typing the following command into the command line:

```
print sendmodule$(lpmp, "ser?")
```

The reply line will give the serial number of the isocratic pump.

Replacing the Isocratic Pump's Firmware

The installation of new firmware is required

- if a new version solves problems of the currently installed version.
- if the version of firmware on the new main board (LPM) after an exchange of the board is older than the one previously installed.

4 Repairing the Pump

To upgrade the isocratic pump's firmware follow the procedures and instructions given on the internet @

<http://www.agilent.com>

section *Service&Support - Chemical Analysis - Technical Support*

<http://www.chem.agilent.com>

section *Technical Support*

to download and install always the newest available version of firmware on your system or call your local service provider for assistance.

Exchanging the Damper

When required

No pressure output or when leaking

Tools required


Screwdriver Pozidriv #1

Wrench 1/4 inch


Parts required

Damper 79835-60005

1 Remove the front cover, top cover and top foam section (see "Replacing the Top Cover and Foam" on page 146).

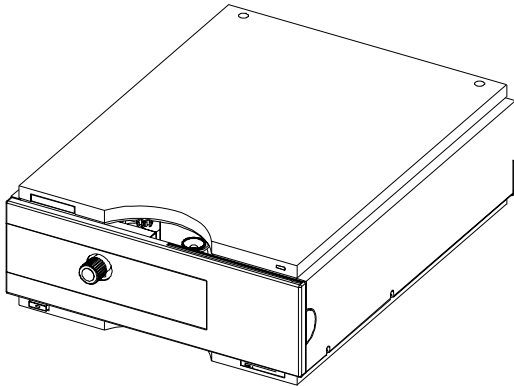


2 Disconnect the two damper capillaries.

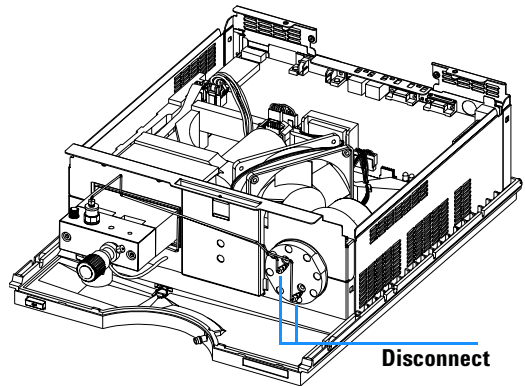


4 Repairing the Pump


3 Loosen the screws of the Z-panel and take it out of the instrument.

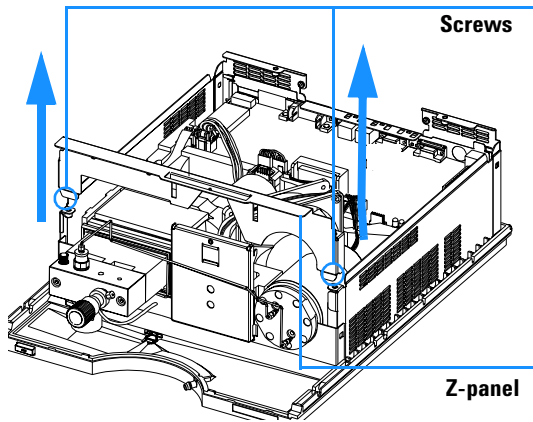


4 Disconnect the damper connector at the main board and lift the damper out of its position.

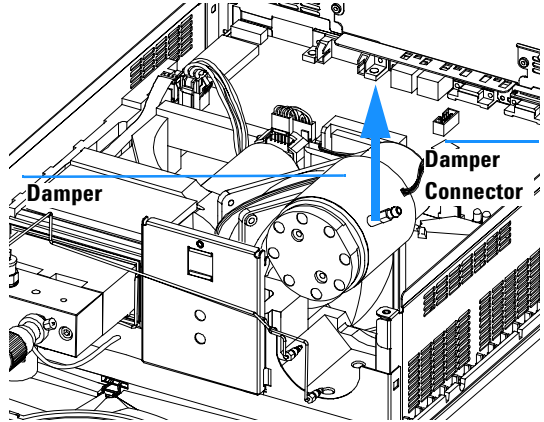


5 Place the new damper into the recess and connect to J24 on the main board (see "Exchanging the Low Pressure Pump Main Board (LPM Board)" on page 121).

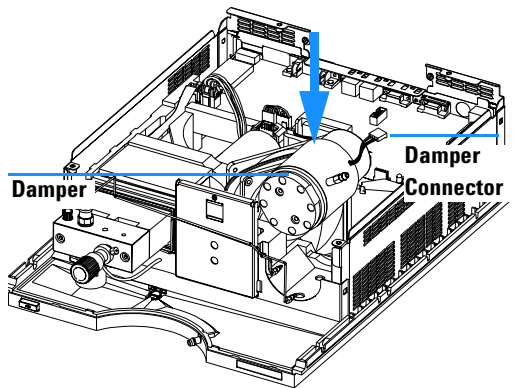


6 Place the Z-panel into position and fix it with the two screws.

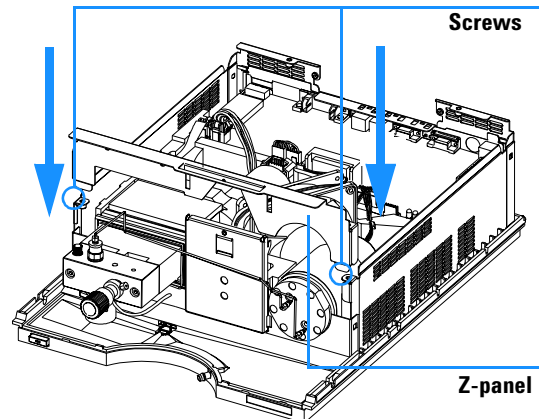

7 Reconnect the two damper capillaries.

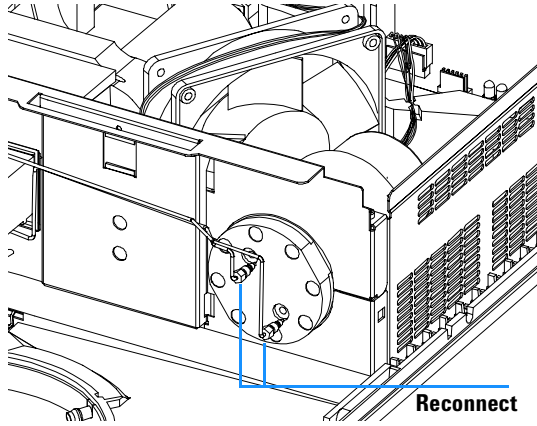

8 Replace the top foam section, optional interface board (if installed), metal cover and top cover. (see ["Replacing the Top Cover and Foam"](#) on page 146). Replace the pump on stack, reconnect all tubings and cables

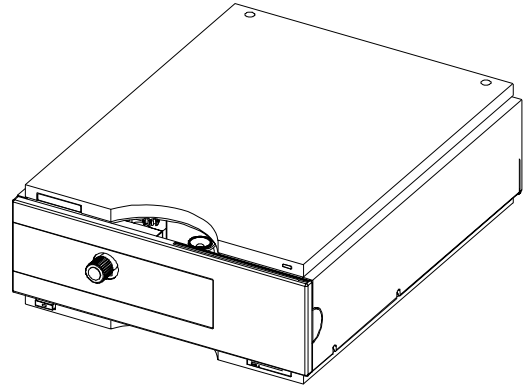

Exchanging the Fan

When required	Fan not running
Tools required	Screwdriver Pozidriv #1
Parts required	Fan, part number 3160-1016

- 1 Switch off the pump at the main power switch, remove all cables and tubings, remove the pump from the stack.
- 2 Remove the front cover, top covers and foam, see [“Removing the Top Cover and Foam”](#) on page 118.
- 3 Disconnect the fan connector at the processor board (J25).
- 4 Slide the cables on the fan housing aside and lift the fan out of the isocratic pump.
- 5 Slide the new fan into its position and connect to J25 on the main board.

CAUTION

Make sure that air flow is directed as indicated (same direction for arrow on the fan and arrow on the bottom foam).

-
- 6 Reinstall foam, top covers and front cover, see [“Replacing the Top Cover and Foam”](#) on page 146.
 - 7 Replace the pump on stack, reconnect all tubings and cables.

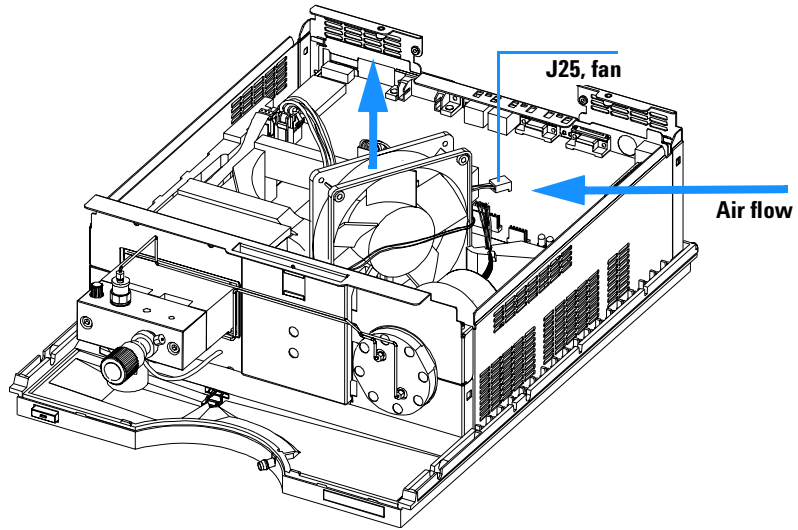


Figure 22 Exchanging the Fan


4 Repairing the Pump

Exchanging the Pump Drive


WARNING

Never start the pump when the pump head is removed. This may damage the pump drive


1 Switch off the pump at the main power switch, remove all cables and tubings, remove the pump from the stack.

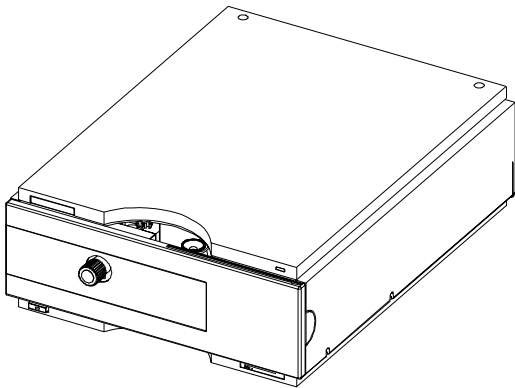


2 Disconnect all capillaries and the waste tube from the pump head and disconnect the active inlet valve connector.

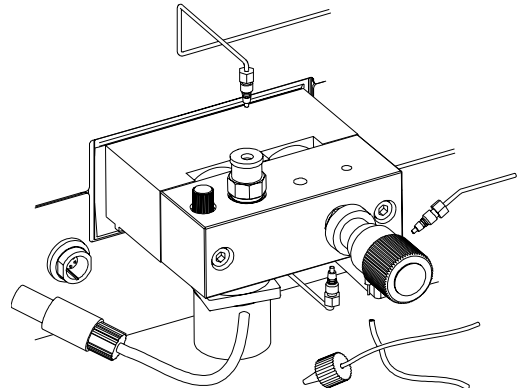


3 Stepwise loosen the two pump-head screws and remove the pump head.

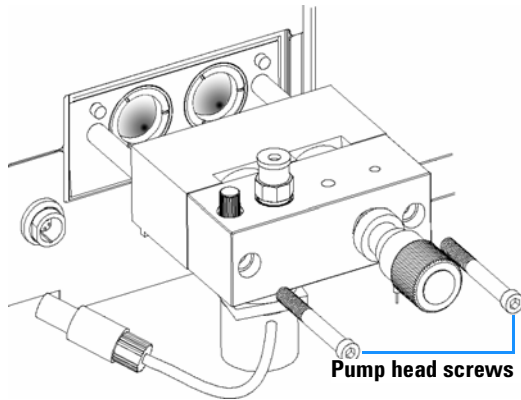


4 Loosen the two screws from the Z-panel and remove it.

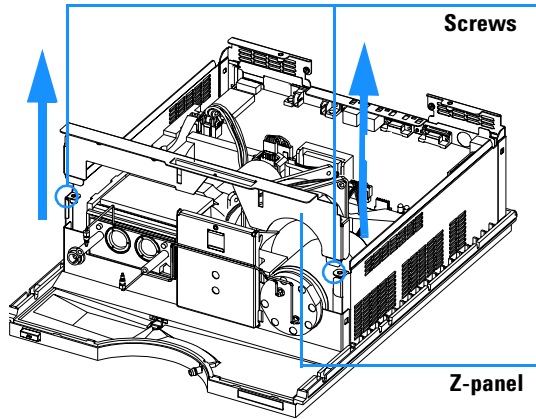

5 Disconnect the pump-drive cables from the main board (J16, J17) and lift the pump drive out of the foam.

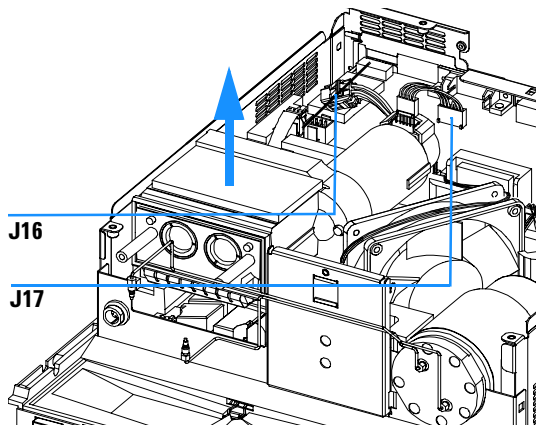


6 Place the new pump drive into the recess in the foam part and connect the cables to the connectors on the main board (J16 motor, J17 encoder).

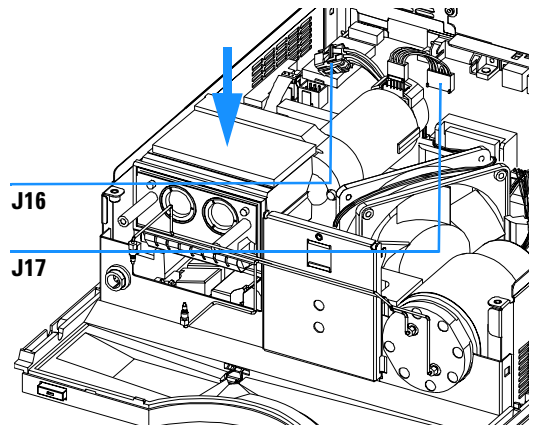


4 Repairing the Pump


7 Replace the Z-panel and fix it with the two screws.

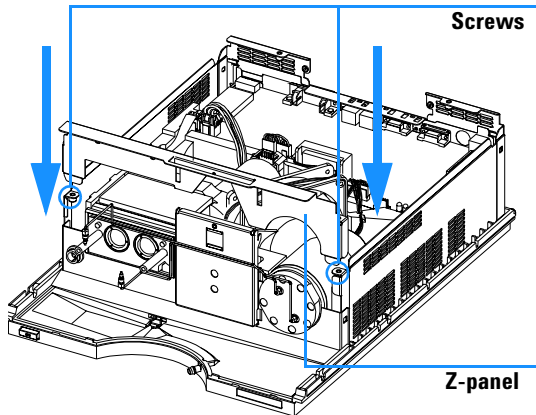


8 Reinstall the pump head and fix with the two screws.

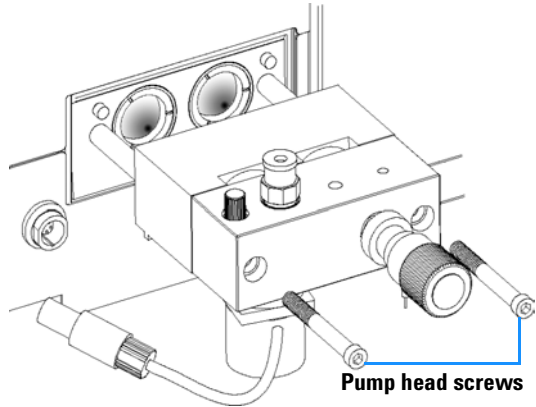

9 Reconnect all capillaries and cables.

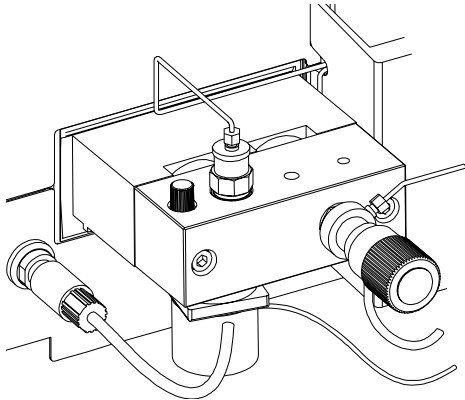


10 Replace the top foam section, optional interface board, front cover, and top cover (see "Replacing the Top Cover and Foam" on page 146).

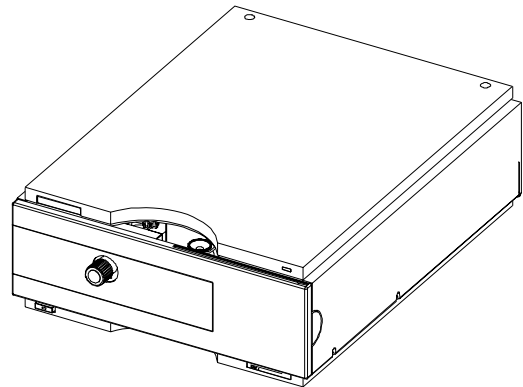


Exchanging the Power Supply

When required	If defective
Tools required	Screwdriver Pozidriv #1
	Wrench 1/4 inch
	Wrench 14 mm
	Wrench 7 mm
	Wrench 5 mm
Parts required	Power supply 0950-2528

1 Remove the pump from stack, remove the front cover, top cover and top foam section (see ["Removing the Top Cover and Foam"](#) on page 118).

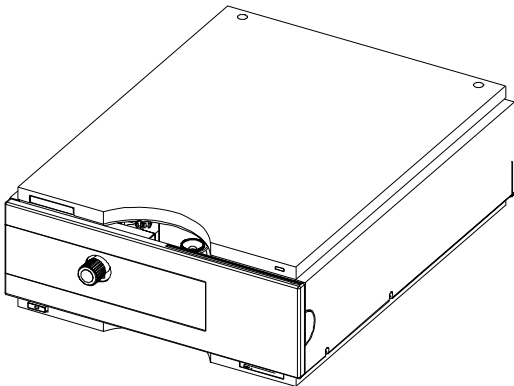


2 Disconnect all capillaries, tubes and connectors from the pump head and the damper.

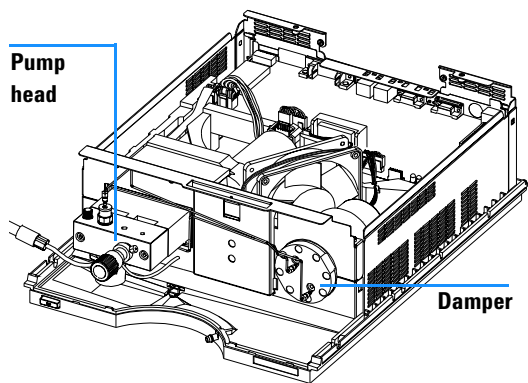


4 Repairing the Pump


3 Loosen the two Z-panel screws and remove it.

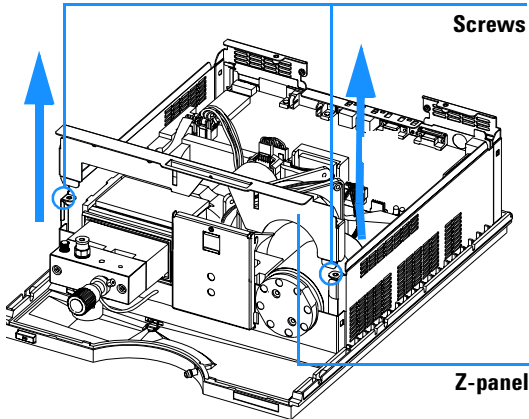


4 Disconnect the connectors of pump assembly (J16, J17), fan (J25) and damper (J24) at the main board and lift the three assemblies out of the foam. Disconnect all remaining connectors at the main board.

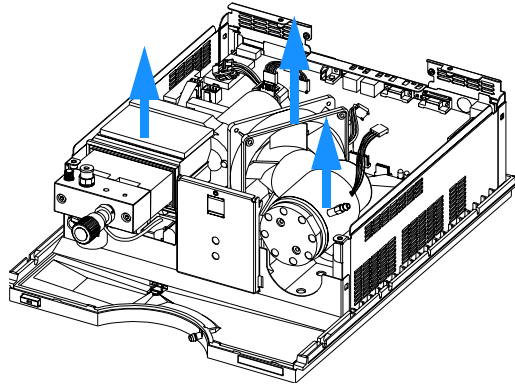


5 Remove the LPM board (see "Exchanging the Low Pressure Pump Main Board (LPM Board)" on page 121).

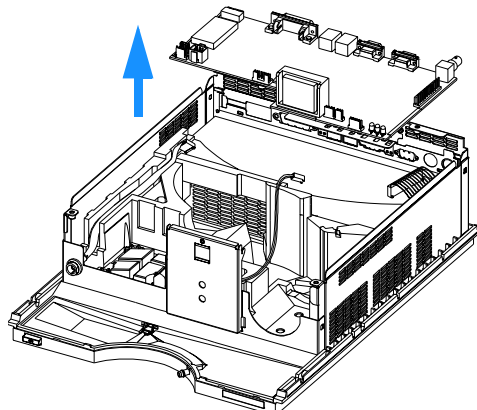


6 Push the leak sensor cable through the recess in the foam and lift the bottom foam out of the isocratic pump.

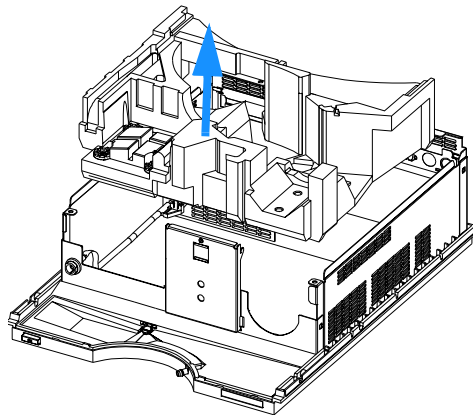


7 Loosen and remove the power supply screws at the rear panel.

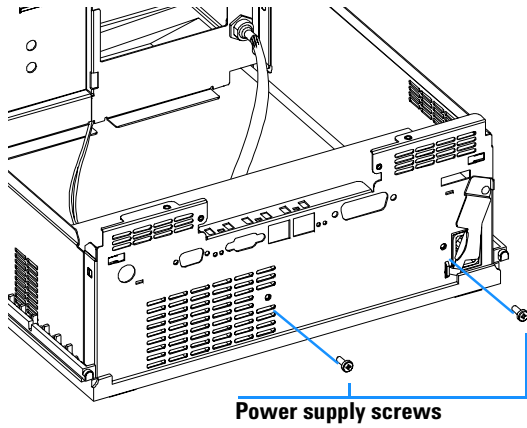


8 Unclip the power supply light pipe from the power supply and pull out the coupler.

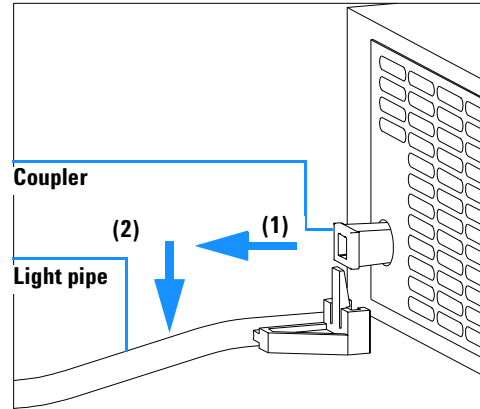

9 Lift the power supply out of the unit.

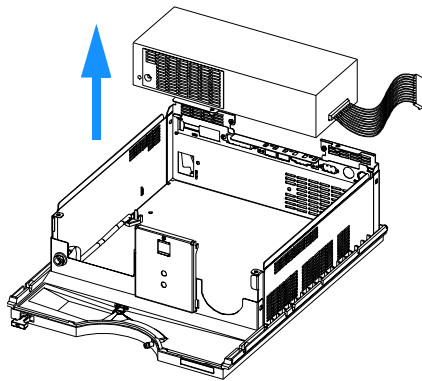


10 Place the new power supply into the isocratic pump and fix the two screws at the back plane.

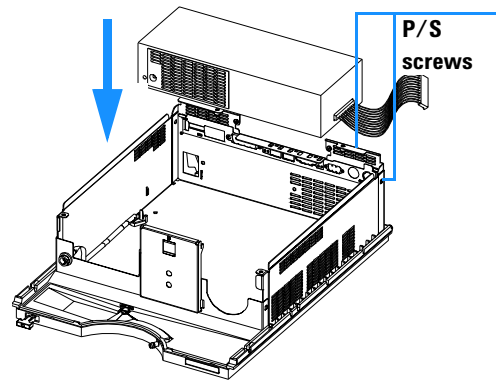


4 Repairing the Pump


11 Install the coupler onto the power supply switch and clip the light pipe back onto the coupler.

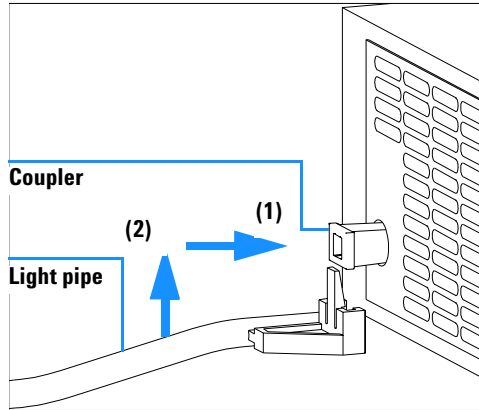


12 Slide the leak sensor cable through the foam and replace the bottom foam.

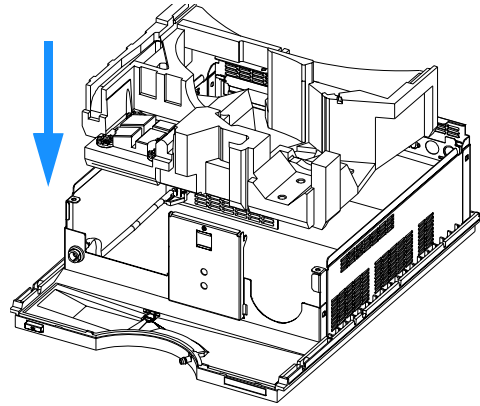


13 Reinstall the main board (see "Exchanging the Low Pressure Pump Main Board (LPM Board)" on page 121).

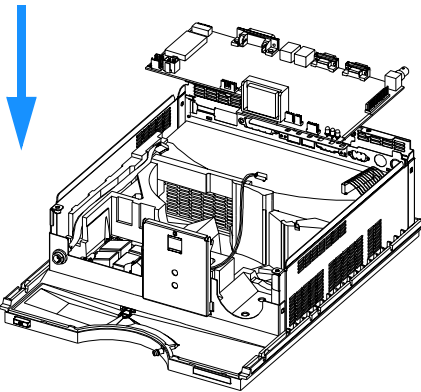


14 Re-install pump assembly, fan and damper into the bottom foam and re-connect to the main board.

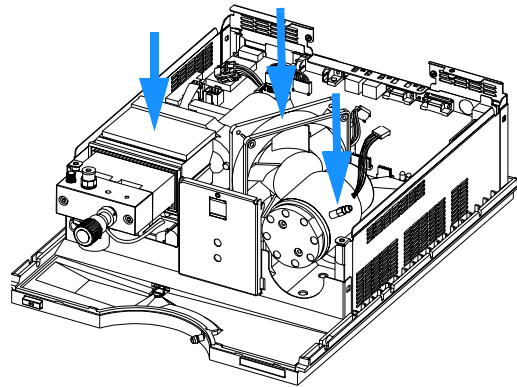


15 Place the Z-panel into its position and tighten the two screws.

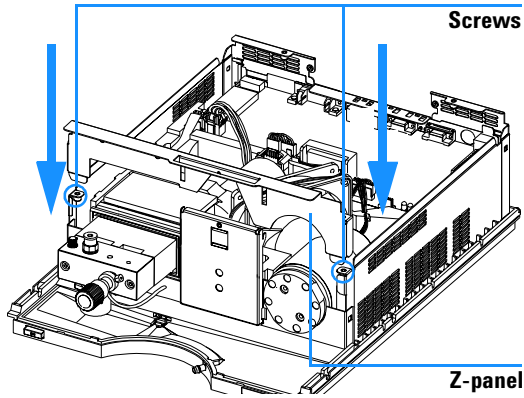

16 Reconnect all capillaries, tubes and cables to the pump head and the damper.

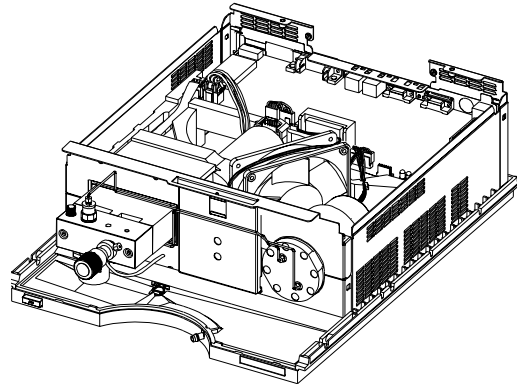

17 Install foam and top cover (see "Replacing the Top Cover and Foam" on page 146). Replace the pump on stack, reconnect all tubings and cables.

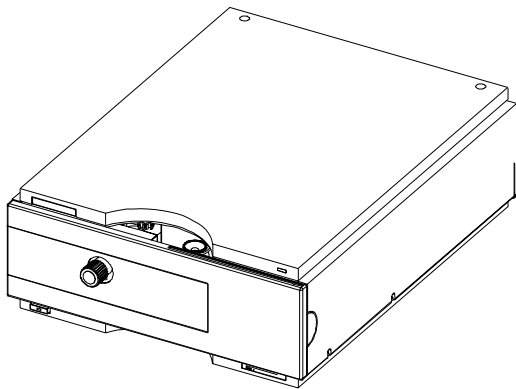

Exchanging the Leak Sensor

When required	Leak messages without leak in the leak pan
Tools required	Screwdriver Pozidriv #1 Wrench 1/4 inch Wrench 14 mm Wrench 7 mm Wrench 5 mm
Parts required	Leak sensor 5061-3356

- 1 Switch off the pump at the main power switch, remove all cables and tubings, remove the pump from the stack.
- 2 Remove the top covers and foam, see [“Removing the Top Cover and Foam”](#) on page 118.
- 3 Remove pump assembly, fan, damper and the bottom foam, see [“Exchanging the Power Supply”](#) on page 137.
- 4 Remove the main board, see [“Exchanging the Low Pressure Pump Main Board \(LPM Board\)”](#) on page 121.
- 5 Unclip the leak pan and place it in front of the isocratic pump.
- 6 Pull the leak sensor out of the leak pan and push the leak sensor cable and connector through the hole in the metal plate.
- 7 Push the connector of the new sensor through the metal plate.
- 8 Place the leak sensor into the leak pan, see [Figure 23](#) and clip the pan back into its position.
- 9 Reinstall the bottom foam. Make sure that the leak sensor cable is not covered by the foam.
- 10 Replace the main board, see [“Exchanging the Low Pressure Pump Main Board \(LPM Board\)”](#) on page 121.
- 11 Install the pump assembly, the fan, the damper and the Z-panel, see [“Exchanging the Power Supply”](#) on page 137. Reconnect all cables and capillaries.
- 12 Replace top foam and top cover, see [“Replacing the Top Cover and Foam”](#) on page 146.
- 13 Replace the pump on stack, reconnect all tubings and cables.

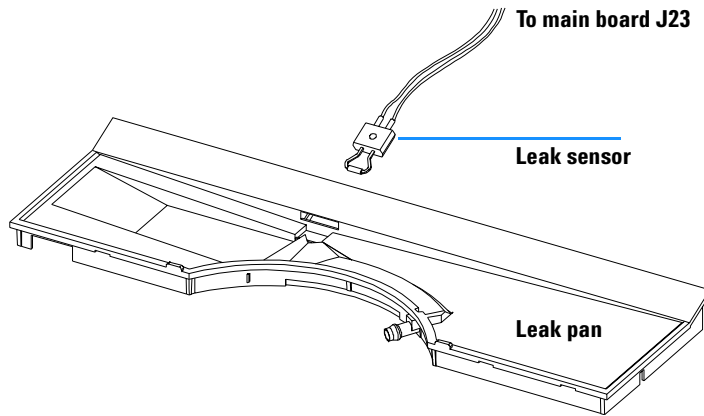


Figure 23 Exchanging the Leak Sensor

4 Repairing the Pump

Exchanging the Status Light Pipe

When required

If part is broken

Tools required

Screwdriver Pozidriv #1


Part required

Status light pipe 5041-8384

Preparations for this procedure

Remove the front cover and top cover, see ["Removing the Top Cover and Foam"](#) on page 118

1 The status light pipe is clipped into the top cover.

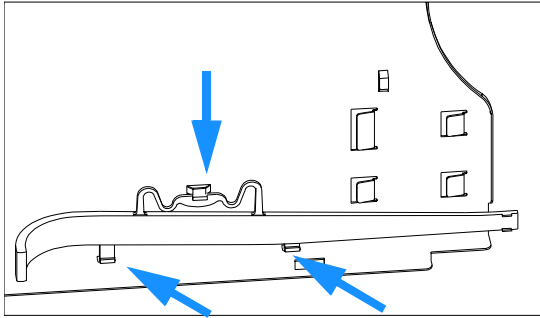

2 Replace the top cover, see ["Replacing the Top Cover and Foam"](#) on page 146.

3 Replace the isocratic pump into the stack and reconnect the cables and capillaries.

4 Turn on the isocratic pump.

Assembling the Main Cover

When required	If cover is broken
Tools required	None
Parts required	Cover kit 5062-8565 (includes base, top, left and right)


NOTE

The cover kit contains all parts, but it is not assembled.


WARNING

In case you insert the left or right side in the opposite position, you may not be able to remove the side from the top part.

1 Place the top part on the bench and insert the left and right side into the top part.

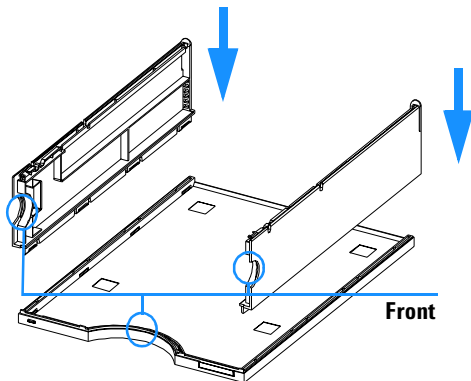

2 Replace the cover.

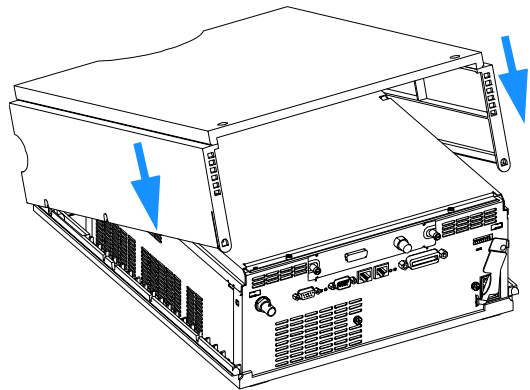

3 Replace the isocratic pump into the stack and reconnect the cables and capillaries.

4 Turn on the isocratic pump.

Replacing the Top Cover and Foam


Tools required

Screwdriver Pozidriv #1


Preparations for this procedure

Make sure that after your repair all assemblies, cables, capillaries and connectors are located in its correct place.


1 Replace the top foam section.

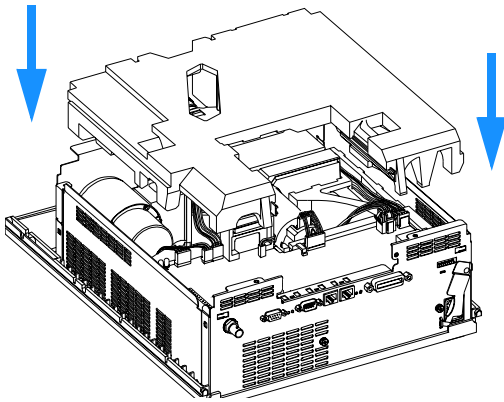


2 Make sure that the foam is installed correctly and is located in the safety light switch.

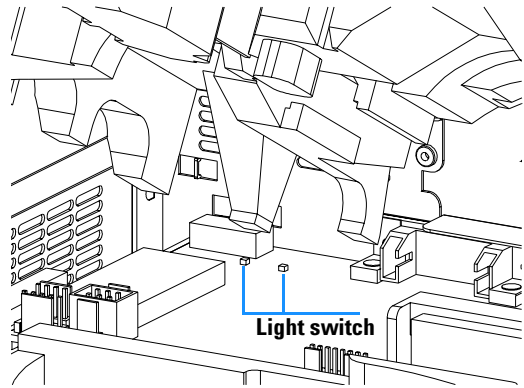


3 Location of foam in the light switch.

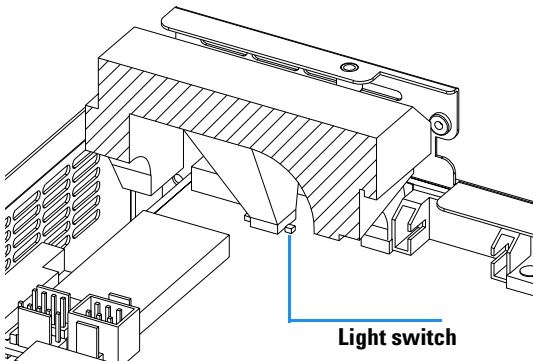


4 Replace the optional interface board.

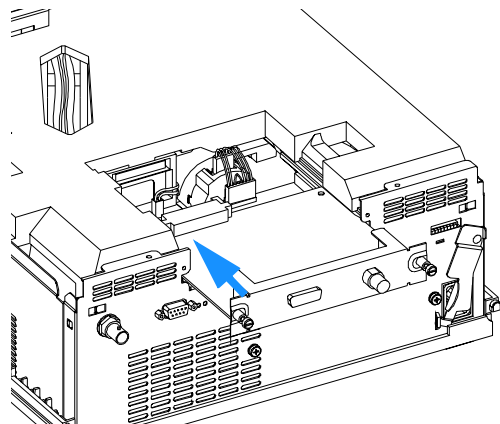


5 Replace the metal cover (slide the metal tabs into place (1) underneath the Z-Panel in the front, then lower the back of the metal plate (2)) and fix the two holding screws.

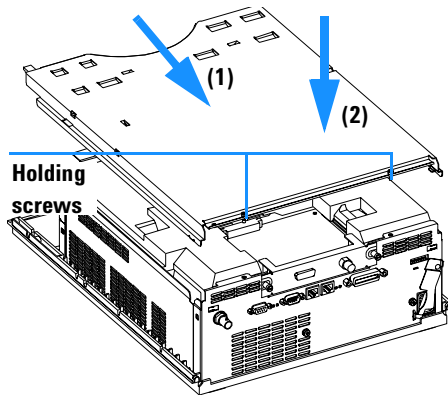


6 Replace the top cover. Replace the pump on stack, reconnect all tubings and cables.

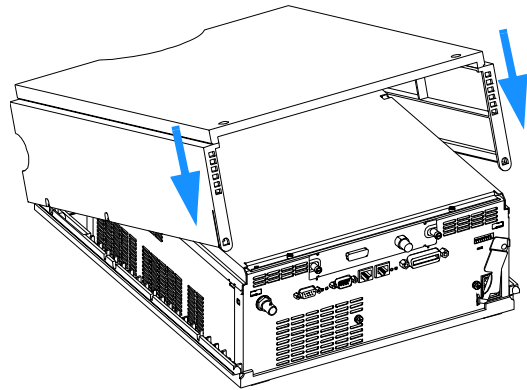

7 Place the isocratic pump back to its position in the stack, replace solvent cabinet and connect the solvent tube to the adapter of the active inlet valve.

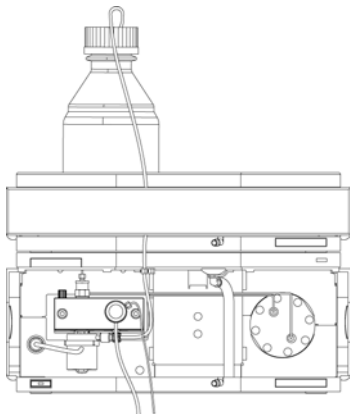

8 Replace the front covers and reconnect the power cable to the isocratic pump. Switch the isocratic pump on.

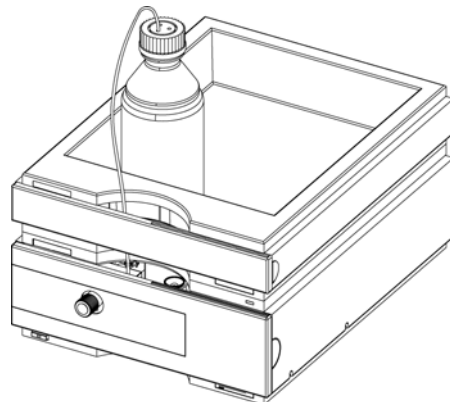

4 Repairing the Pump



5 Parts and Materials

Overview of Main Assemblies	150
Control Module (B-Version)	153
Solvent Cabinet	154
Bottle Head Assembly	155
Hydraulic Path	156
Cover Parts	157
Sheet Metal Kit	158
Foam Parts	159
Power and Status Light Pipes	160
Leak Parts	161
Pump Head Assembly	162
Pump Head Assembly with Seal Wash Option	164
Outlet Ball Valve Assembly	166
Purge Valve Assembly	167
Active Inlet Valve Assembly	168
Accessory Kit G1311-68075	169
Seal Wash Option Kit 01018-68722	170
Cable Overview	171
RS-232 Cable Kit	186
LAN Cables	187



Overview of Main Assemblies

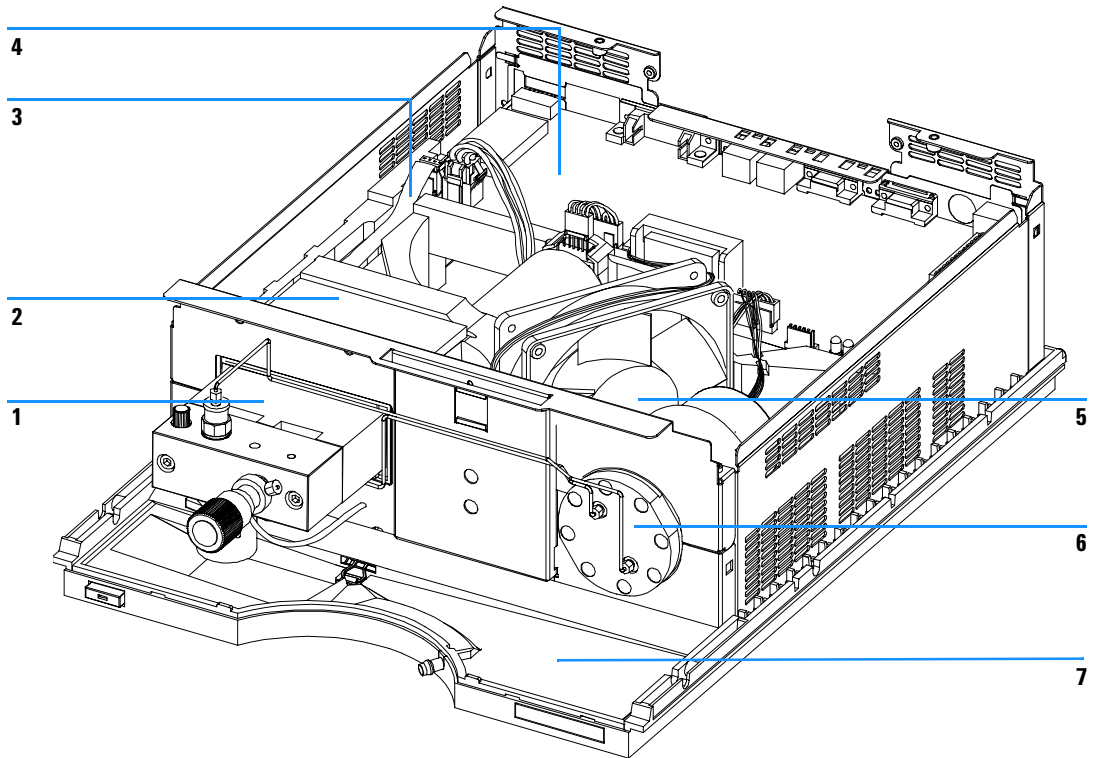


Figure 24 Overview of Main Assemblies (Front View)

Table 7 Repair Parts — Pump Housing and Main Assemblies

Item	Description	Part Number
1	Pump head, see page 162	G1311-60004
2	Pump drive assembly	G1311-60001
	Exchange assembly — pump drive	G1311-69001

Table 7 Repair Parts — Pump Housing and Main Assemblies (continued)

Item	Description	Part Number
3	Cable assembly — AIV to main board	G1311-61601
4	Low-pressure pump main board (LPM) Exchange assembly — LPM board	G1311-66520 G1311-69520
5	Fan assembly	3160-1016
6	Damping unit	79835-60005
7	Leak pan — pump	5041-8390

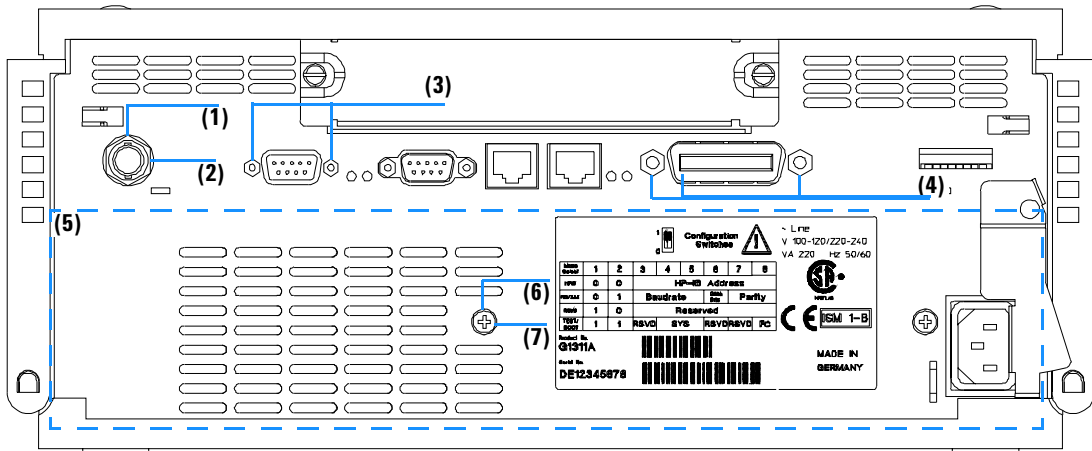


Figure 25 Overview of Main Assemblies (Rear View)

Table 8 Repair Parts - Pump Housing and Main Assemblies (Rear View)

Item	Description	Part Number
1	Nut M14 — analog output	2940-0256
2	Washer — analog output	2190-0699
3	Standoff — remote connector	1251-7788

Table 8 Repair Parts - Pump Housing and Main Assemblies (Rear View) (continued)

Item	Description	Part Number
4	Standoff — GPIB connector	0380-0643
5	Power supply (behind rear panel)	0950-2528
6	Screw, M4, 7 mm lg — power supply	0515-0910
7	Washer — power supply	2190-0409

Control Module (B-Version)

Table 9 Control Module

Item	Description	Part Number
	Control module, replacement part including cable	G1323-67001
	Plastic Housing Kit, includes front, back and a clamp	5062-8583
	CAN cable, Agilent 1100 module to control module	G1323-81600

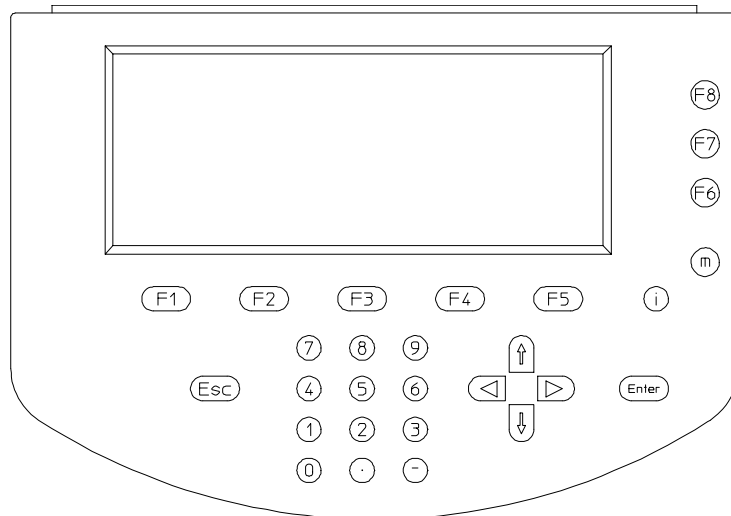


Figure 26 Control Module.

Solvent Cabinet

Table 10 Solvent Cabinet Parts

Item	Description	Part Number
1	Solvent cabinet, including all plastic parts	5062-8581
2	Name plate, Agilent 1100	5042-1381
3	Front panel, solvent cabinet	5062-8580
4	Leak pan, solvent cabinet	5042-1307
5	Bottle amber	9301-1450
6	Bottle transparent	9301-1430
7	Bottle-head assembly, see page 155	G1311-60003

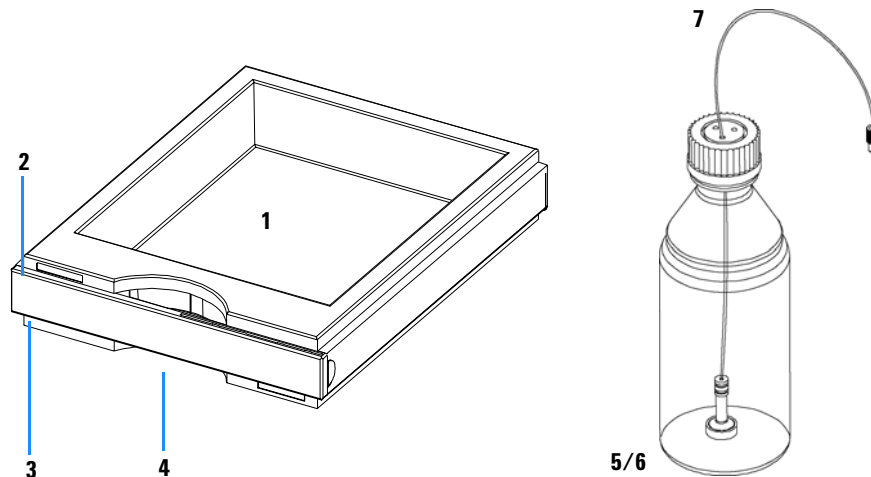


Figure 27 Solvent Cabinet Parts

Bottle Head Assembly

Table 11 Bottle-Head Assembly Parts

Item	Description	Part Number
	Complete assembly	G1311-60003
1	Ferrules with lock ring	5063-6598 (10x)
2	Tube screw	5063-6599 (10x)
3	Wire marker	No part number
4	Solvent tubing, 5 m	5062-2483
5	Frit adapter (pack of 4)	5062-8517
6	Solvent inlet filter 20 μ m	5041-2168

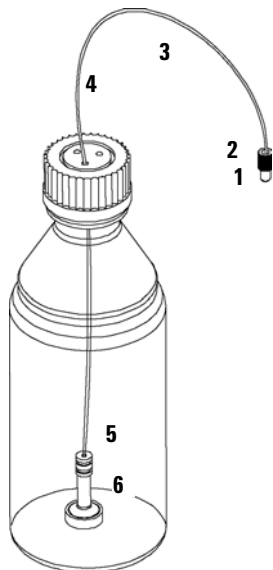


Figure 28 Bottle-Head Assembly Parts

Hydraulic Path

Table 12 Hydraulic Path

Item	Description	Part Number
1	Capillary, plunger 1 to damper	G1311-67301
2	Bottle-head assembly	G1311-60003
3	Capillary, damper to plunger 2	G1311-67300
4	Outlet capillary, pump to injector device	G1312-67305
	Outlet Capillary, pump to thermostatable autosampler	G1329-87300
5	Waste tube, 5 m (reorder pack)	5062-2461
6	Adapter, AIV to solvent inlet tubes	0100-1847

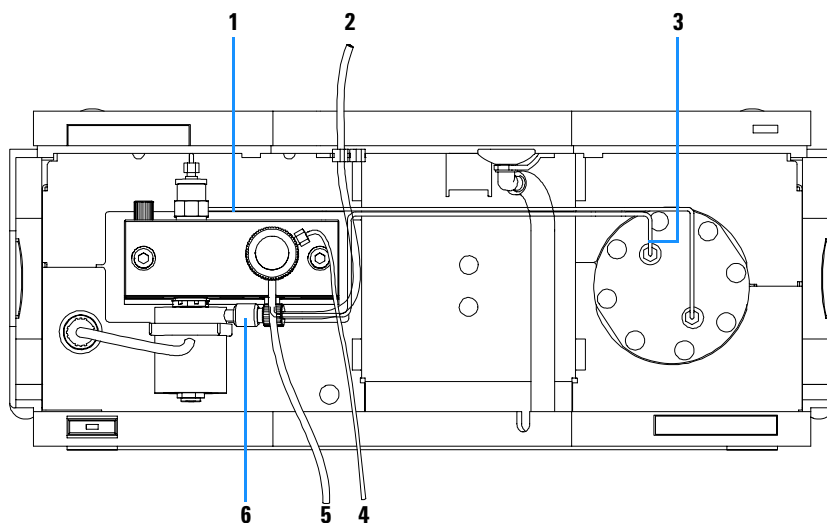


Figure 29 Hydraulic Flow Path of the Isocratic Pump

Cover Parts

Table 13 Cover Parts

Item	Description	Part Number
1	Cover kit (includes top, both sides, base)	5062-8565
2	Front plate	5062-8566
3	Logo plate, Agilent 1100	5042-1381

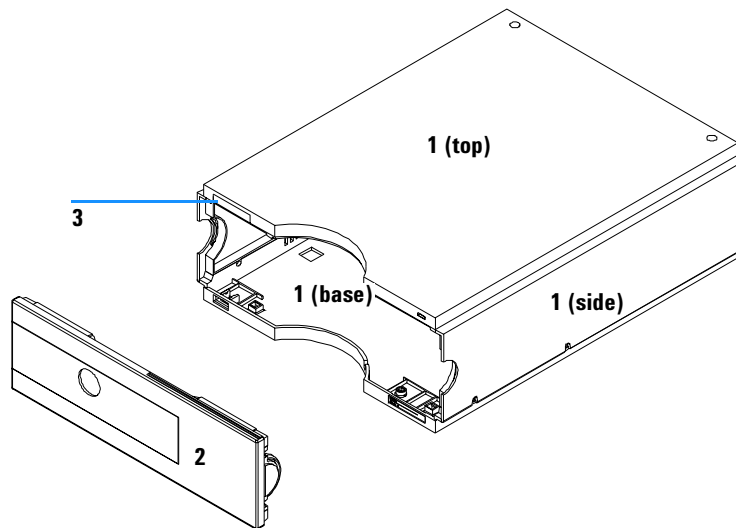


Figure 30 Cover Parts

Sheet Metal Kit

Table 14 Sheet Metal Kit

Item	Description	Part Number
1	Sheet metal kit, includes top, base and Z-panel	G1311-68701
2	Screw, for cover and Z-Panel	5022-2112
3	Board cover	5001-3772

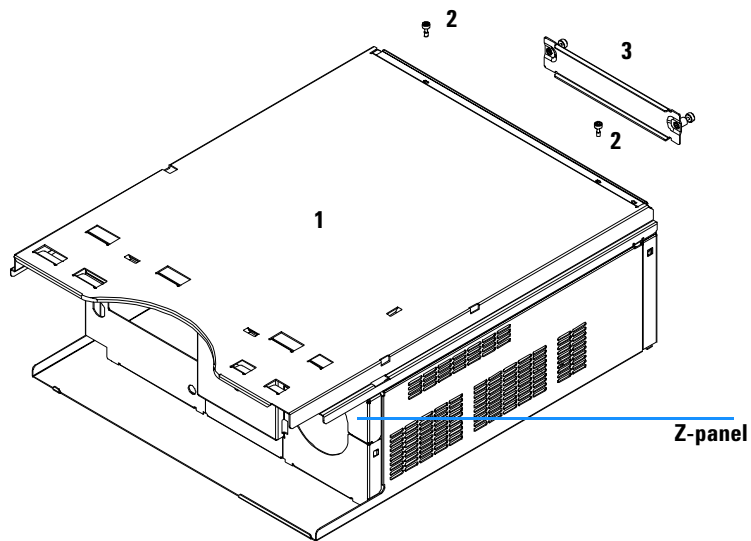


Figure 31 Sheet Metal Kit

Foam Parts

Table 15 Foam Parts

Item	Description	Part Number
1	Foam kit (includes upper and lower foam)	G1311-68702
2	Bushing, for pump drive	1520-0404
3	Board guides	5041-8395

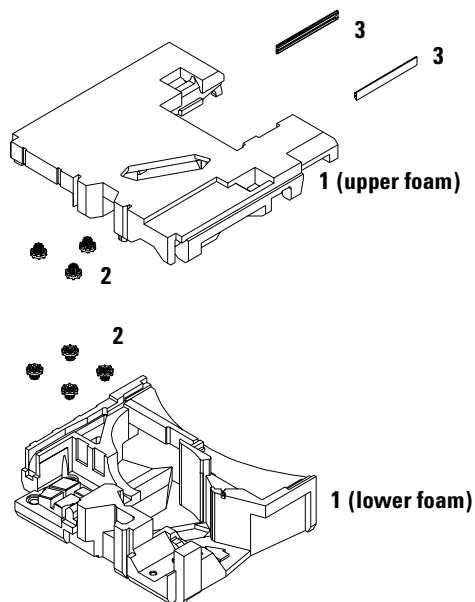


Figure 32 Foam Parts

Power and Status Light Pipes

Table 16 Power and Status Light Pipes

Item	Description	Part Number
1	Power switch coupler	5041-8383
2	Light pipe — power switch	5041-8382
3	Power switch button	5041-8381
4	Light pipe — status lamp	5041-8384

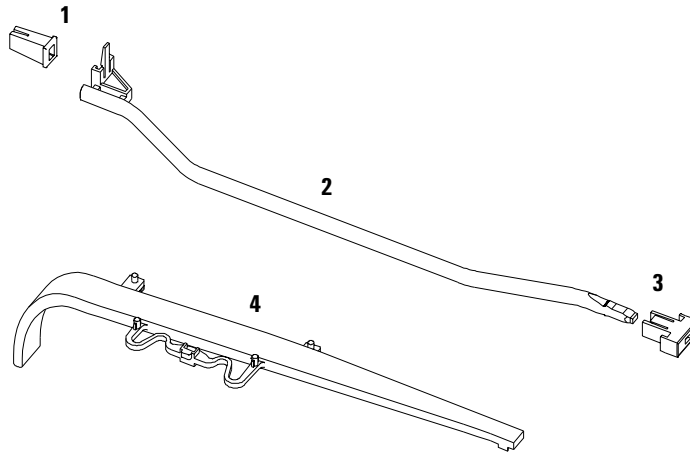


Figure 33 Power and Status Light Pipes

Leak Parts

Table 17 Leak Parts

Item	Description	Part Number
1	Leak sensor	5061-3356
2	Tube clip	5041-8387
3	Leak pan, pump	5041-8390
4	Leak funnel	5041-8388
5	Holder, leak funnel	5041-8389
6	Corrugated waste tube (reorder pack), 5m	5062-2463

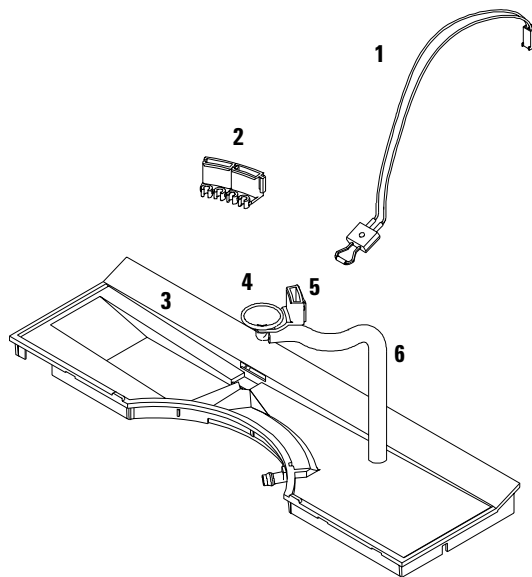


Figure 34 Leak Parts

Pump Head Assembly

Table 18 Pump Head Assembly

Item	Description	Part Number
	Complete assembly, including items marked with *	G1311-60004
1*	Sapphire plunger	5063-6586
2*	Plunger housing (including spring)	G1311-60002
3*	Support ring	5001-3739
4*	Seal (pack of 2) <u>or</u> Seal (pack of 2), for normal phase applications	5063-6589 0905-1420
5*	Pump chamber housing	G1311-25200
6	Active inlet valve (complete with cartridge)	G1312-60010
	Replacement cartridge for active inlet valve	5062-8562
7	Outlet ball valve	G1311-60012
8*	Screw lock	5042-1303
9	Purge valve assembly	G1311-60009
10*	Screw M5, 60 mm lg	0515-2118

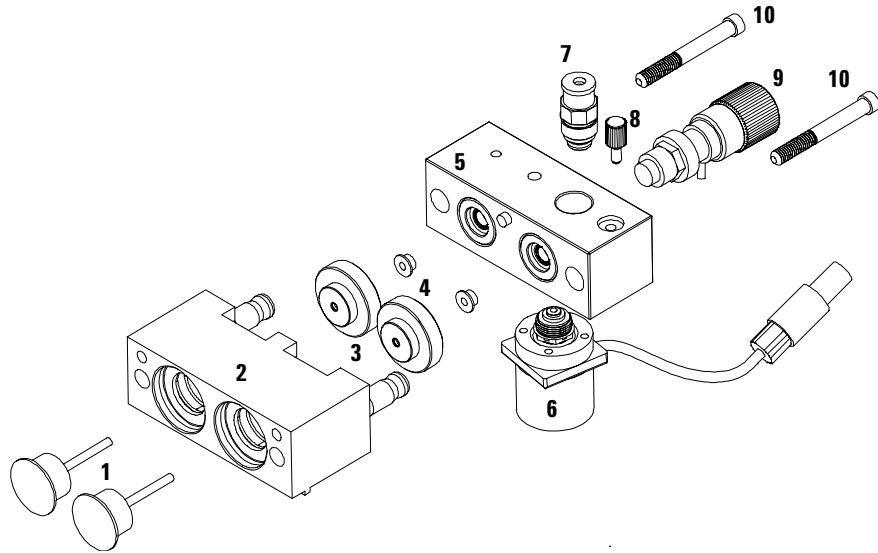


Figure 35 Pump Head Assembly

Pump Head Assembly with Seal Wash Option

Table 19 Pump Head Assembly with Seal Wash Option

Item	Description	Part Number
	Complete assembly, including parts marked with *	G1311-60005
1*	Sapphire plunger	5063-6586
2*	Plunger housing (including spring)	G1311-60002
3*	Support ring, seal wash	5062-2465
4*	Secondary seal	0905-1175
5*	Wash tube (1.0 m)	0890-1764
6*	Gasket, seal wash (pack of 6)	5062-2484
7*	Seal keeper	5001-3743
8*	Seal (pack of 2) or Seal (pack of 2), for normal phase applications	5063-6589 0905-1420
9*	Pump chamber housing	G1311-25200
10	Active inlet valve	G1312-60010
	Replacement cartridge for active inlet valve	5062-8562
11	Outlet ball valve (complete with cartridge)	G1311-60012
12*	Screw lock	5042-1303
13	Purge valve	G1311-60009
14*	Screw M5, 60 mm lg	0515-2118
	Seal wash upgrade kit (see page 170)	01018-68722

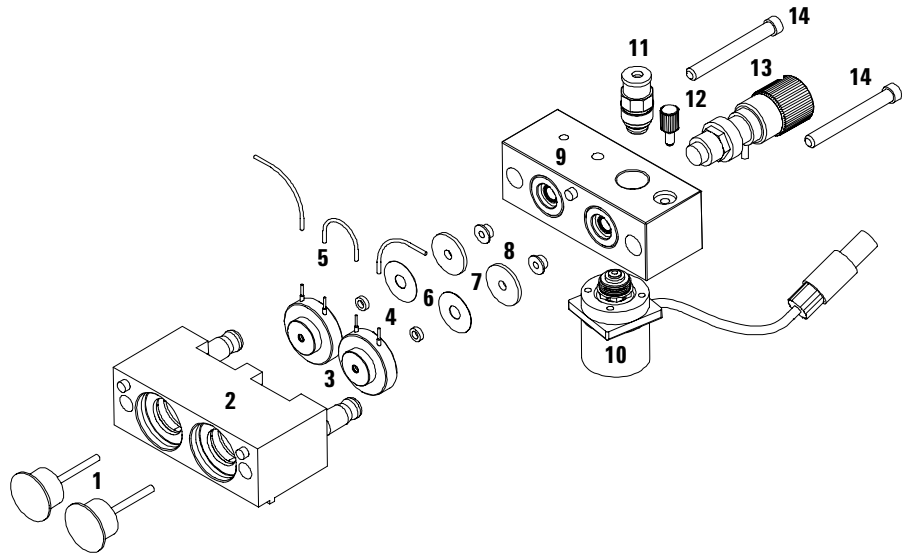


Figure 36 Pump Head with Seal Wash Option

Outlet Ball Valve Assembly

Table 20 Outlet Ball Valve Assembly

Item	Description	Part Number
	Outlet ball valve — complete assembly	G1311-60012
1	Socket cap	5042-1345
2	Outlet valve housing screw	01018-22410
3	Gold seal, outlet	5001-3707
4	Cap (pack of 4)	5062-2485

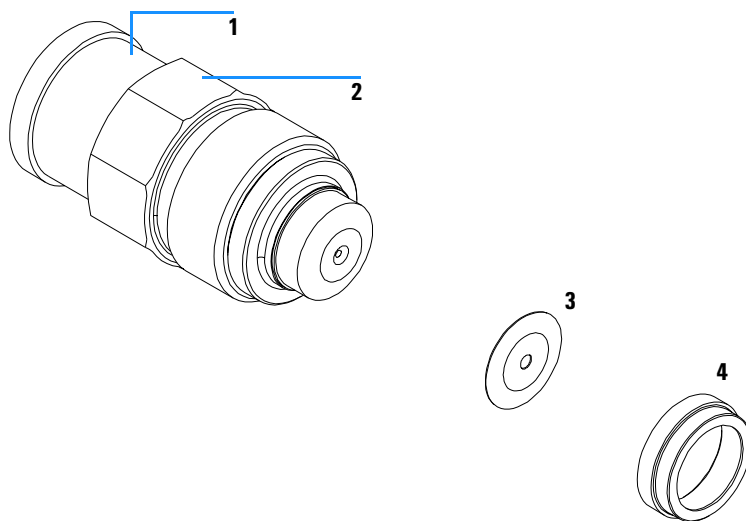


Figure 37 Outlet Ball Valve Assembly

Purge Valve Assembly

Table 21 Purge-Valve Assembly

Item	Description	Part Number
	Purge valve — complete assembly	G1311-60009
1	Valve body	No part number
2	PTFE frit (pack of 5)	01018-22707
3	Gold seal	5001-3707
4	Cap (pack of 4)	5062-2485

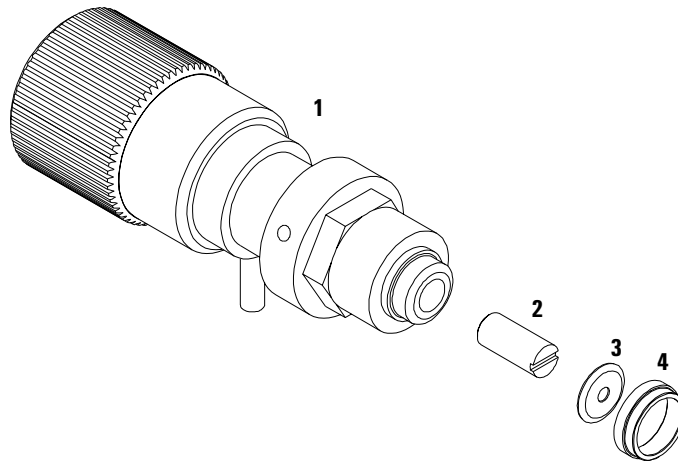


Figure 38 Purge-Valve Assembly

Active Inlet Valve Assembly

Table 22 Active Inlet Valve Assembly

Item	Description	Part Number
	Active inlet valve — complete assembly	G1312-60010
1	Valve body	No part number
2	Valve cartridge	5062-8562

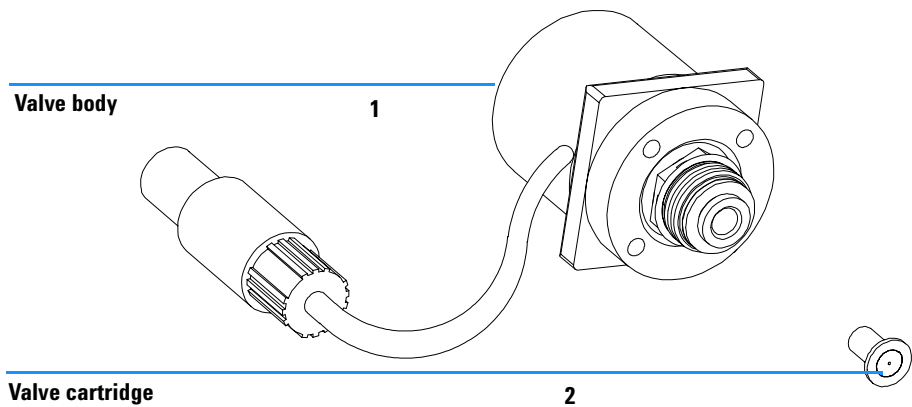


Figure 39 Active Inlet Valve Assembly

Accessory Kit G1311-68075

Table 23 Tools and Accessories

Description	Part Number
Wrench 14 mm	8710-1924
Seal insert tool	01018-23702
PTFE Frit (pack of 5)	01018-22707
Corrugated waste tube (1.2 m)	no PN
Corrugated waste tube (reorder number), 5m	5062-2463
Velocity regulator (reorder number, 3)	5062-2486
ESD wrist strap	9300-1408
Hex key 4mm	8710-2392
Wrench 1/4 – 5/16 inch	8710-0510
Capillary, pump to injection device, 600 mm lg, ID 0.17 mm	G1312-67305

Seal Wash Option Kit **01018-68722**

Table 24 Seal Wash Option

Description	Part Number
Support ring, seal wash (pack of 2)	5062-2465
Secondary seal (pre-installed in support ring)	0905-1175
Seal keeper (pack of 2)	5001-3743
Wash tube (1m)	0890-1764
Velocity regulator [*]	5062-2486
Seals insert tool	01018-23702
Seal (pack of 2)	5063-6589
Syringe ^{**}	5062-8534
Syringe adapter	0100-1681
Knife	no PN
Sanding Paper	no PN

* Reorder number (pack of 3)

** Reorder number (pack of 10)

Cable Overview

WARNING

Never use cables other than the ones supplied by Agilent Technologies to ensure proper functionality and compliance with safety or EMC regulations.


Table 25 Cables Overview

Type	Description	Part Number
Analog cables	3390/2/3 integrators	01040-60101
	3394/6 integrators	35900-60750
	Agilent 35900A A/D converter	35900-60750
	General purpose (spade lugs)	01046-60105
Remote cables	3390 integrator	01046-60203
	3392/3 integrators	01046-60206
	3394 integrator	01046-60210
	3396A (Series I) integrator	03394-60600
	3396 Series II / 3395A integrator, see page 178	
	3396 Series III / 3395B integrator	03396-61010
	HP 1050 modules / HP 1046A FLD	5061-3378
	HP 1046A FLD	5061-3378
	Agilent 35900A A/D converter	5061-3378
	HP 1040 diode-array detector	01046-60202
	HP 1090 liquid chromatographs	01046-60202
	Signal distribution module	01046-60202
BCD cables	3392/3 integrators	18594-60510

Table 25 Cables Overview (continued)

Type	Description	Part Number
	3396 integrator	03396-60560
	General purpose (spade Lugs)	18594-60520
Auxiliary	Agilent 1100 Series vacuum degasser	G1322-61600
CAN cables	Agilent 1100 module to module, 0.5m lg	5181-1516
	Agilent 1100 module to module, 1m lg	5181-1519
	Agilent 1100 module to control module	G1323-81600
External contacts	Agilent 1100 Series interface board to general purpose	G1103-61611
GPIB cable	Agilent 1100 module to ChemStation, 1 m	10833A
	Agilent 1100 module to ChemStation, 2 m	10833B
RS-232 cable	Agilent 1100 module to a computer This kit contains a 9-pin female to 9-pin female Null Modem (printer) cable and one adapter.	34398A
LAN cable	Twisted pair cross over LAN cable, 10 feet long (for point to point connection)	5183-4649
	Category 5 UTP cable, 8 m long (for hub connections)	G1530-61480

Analog Cables




One end of these cables provides a BNC connector to be connected to Agilent 1100 Series modules. The other end depends on the instrument to which connection is being made.


Agilent 1100 to 3390/2/3 Integrators

Connector 01040-60101	Pin 3390/2/3	Pin Agilent 1100	Signal Name
	1	Shield	Ground
	2		Not connected
	3	Center	Signal +
	4		Connected to pin 6
	5	Shield	Analog -
	6		Connected to pin 4
	7		Key
	8		Not connected


Agilent 1100 to 3394/6 Integrators

Connector 35900-60750	Pin 3394/6	Pin Agilent 1100	Signal Name
	1		Not connected
	2	Shield	Analog -
	3	Center	Analog +

Agilent 1100 to BNC Connector

Connector 8120-1840	Pin BNC	Pin Agilent 1100	Signal Name
	Shield	Shield	Analog -
	Center	Center	Analog +

Agilent 1100 to General Purpose



Connector 01046-60105	Pin 3394/6	Pin Agilent 1100	Signal Name
	1		Not connected
	2	Black	Analog -
	3	Red	Analog +

Remote Cables




One end of these cables provides a Agilent Technologies APG (Analytical Products Group) remote connector to be connected to Agilent 1100 Series modules. The other end depends on the instrument to be connected to.


Agilent 1100 to 3390 Integrators

Connector 01046-60203	Pin 3390	Pin Agilent 1100	Signal Name	Active (TTL)
	2	1 - White	Digital ground	
	NC	2 - Brown	Prepare run	Low
	7	3 - Gray	Start	Low
	NC	4 - Blue	Shut down	Low
	NC	5 - Pink	Not connected	
	NC	6 - Yellow	Power on	High
	NC	7 - Red	Ready	High
	NC	8 - Green	Stop	Low
	NC	9 - Black	Start request	Low

Agilent 1100 to 3392/3 Integrators

Connector 01046-60206	Pin 3392/3	Pin Agilent 1100	Signal Name	Active (TTL)
 <p>4 - Key</p>	3	1 - White	Digital ground	
	NC	2 - Brown	Prepare run	Low
	11	3 - Gray	Start	Low
	NC	4 - Blue	Shut down	Low
	NC	5 - Pink	Not connected	
	NC	6 - Yellow	Power on	High
	9	7 - Red	Ready	High
	1	8 - Green	Stop	Low
	NC	9 - Black	Start request	Low


Agilent 1100 to 3394 Integrators

Connector 01046-60210	Pin 3394	Pin Agilent 1100	Signal Name	Active (TTL)
	9	1 - White	Digital ground	
	NC	2 - Brown	Prepare run	Low
	3	3 - Gray	Start	Low
	NC	4 - Blue	Shut down	Low
	NC	5 - Pink	Not connected	
	NC	6 - Yellow	Power on	High
	5,14	7 - Red	Ready	High
	6	8 - Green	Stop	Low
	1	9 - Black	Start request	Low
	13, 15		Not connected	

NOTE

START and STOP are connected via diodes to pin 3 of the 3394 connector.


Agilent 1100 to 3396A Integrators

Connector 03394-60600	Pin 3394	Pin Agilent 1100	Signal Name	Active (TTL)
	9	1 - White	Digital ground	
	NC	2 - Brown	Prepare run	Low
	3	3 - Gray	Start	Low
	NC	4 - Blue	Shut down	Low
	NC	5 - Pink	Not connected	
	NC	6 - Yellow	Power on	High
	5,14	7 - Red	Ready	High
	1	8 - Green	Stop	Low
	NC	9 - Black	Start request	Low
	13, 15		Not connected	


Agilent 1100 to 3396 Series II / 3395A Integrators

Use the cable [03394-60600](#) and cut pin #5 on the integrator side. Otherwise the integrator prints START; not ready.


Agilent 1100 to 3396 Series III / 3395B Integrators

Connector 03396-61010	Pin 33XX	Pin Agilent 1100	Signal Name	Active (TTL)
	9	1 - White	Digital ground	
	NC	2 - Brown	Prepare run	Low
	3	3 - Gray	Start	Low
	NC	4 - Blue	Shut down	Low
	NC	5 - Pink	Not connected	
	NC	6 - Yellow	Power on	High
	14	7 - Red	Ready	High
	4	8 - Green	Stop	Low
	NC	9 - Black	Start request	Low
	13, 15		Not connected	


Agilent 1100 to HP 1050, HP 1046A or Agilent 35900 A/D Converters

Connector 5061-3378	Pin HP 1050/....	Pin Agilent 1100	Signal Name	Active (TTL)
	1 - White	1 - White	Digital ground	
	2 - Brown	2 - Brown	Prepare run	Low
	3 - Gray	3 - Gray	Start	Low
	4 - Blue	4 - Blue	Shut down	Low
	5 - Pink	5 - Pink	Not connected	
	6 - Yellow	6 - Yellow	Power on	High
	7 - Red	7 - Red	Ready	High
	8 - Green	8 - Green	Stop	Low
	9 - Black	9 - Black	Start request	Low

Agilent 1100 to HP 1090 LC, HP 1040 DAD or Signal Distribution Module

Connector 01046-60202	Pin HP 1090	Pin Agilent 1100	Signal Name	Active (TTL)
 <p>5 - Key</p>	1	1 - White	Digital ground	
	NC	2 - Brown	Prepare run	Low
	4	3 - Gray	Start	Low
	7	4 - Blue	Shut down	Low
	8	5 - Pink	Not connected	
	NC	6 - Yellow	Power on	High
	3	7 - Red	Ready	High
	6	8 - Green	Stop	Low
	NC	9 - Black	Start request	Low

Agilent 1100 to General Purpose

Connector 01046-60201	Pin Universal	Pin Agilent 1100	Signal Name	Active (TTL)
		1 - White	Digital ground	
		2 - Brown	Prepare run	Low
		3 - Gray	Start	Low
		4 - Blue	Shut down	Low
		5 - Pink	Not connected	
		6 - Yellow	Power on	High
		7 - Red	Ready	High
		8 - Green	Stop	Low
		9 - Black	Start request	Low

BCD Cables




One end of these cables provides a 15-pin BCD connector to be connected to the Agilent 1100 Series modules. The other end depends on the instrument to be connected to.

Agilent 1100 to 3392/3 Integrators


Connector 18584-60510	Pin 3392/3	Pin Agilent 1100	Signal Name	BCD Digit
	10	1	BCD 5	20
	11	2	BCD 7	80
	3	3	BCD 6	40
	9	4	BCD 4	10
	7	5	BCD 0\	1
	5	6	BCD 3	8
	12	7	BCD 2	4
	4	8	BCD 1	2
	1	9	Digital ground	
	2	15	+ 5 V	Low

6 - Key


Agilent 1100 to 3396 Integrators

Connector 03396-60560	Pin 3392/3	Pin Agilent 1100	Signal Name	BCD Digit
	1	1	BCD 5	20
	2	2	BCD 7	80
	3	3	BCD 6	40
	4	4	BCD 4	10
	5	5	BCD 0\	1
	6	6	BCD 3	8
	7	7	BCD 2	4
	8	8	BCD 1	2
	9	9	Digital ground	
	NC	15	+ 5 V	Low

Agilent 1100 to General Purpose


Connector 18594-60520	Wire Color	Pin Agilent 1100	Signal Name	BCD Digit
	Green	1	BCD 5	20
	Violet	2	BCD 7	80
	Blue	3	BCD 6	40
	Yellow	4	BCD 4	10
	Black	5	BCD 0\	1
	Orange	6	BCD 3	8
	Red	7	BCD 2	4
	Brown	8	BCD 1	2
	Gray	9	Digital ground	
	White	15	+5 Vt	Low

Auxiliary Cable




One end of this cable provides a modular plug to be connected to the Agilent 1100 Series vacuum degasser. The other end is for general purpose.

Agilent 1100 Series Degasser to general purposes

Connector G1322-81600	Color	Pin Agilent 1100	Signal Name
	White	1	Ground
	Brown	2	Pressure signal
	Green	3	
	Yellow	4	
	Grey	5	DC + 5 V IN
	Pink	6	Vent


CAN Cable



Both ends of this cable provide a modular plug to be connected to Agilent 1100 Series module's CAN-bus connectors.

Agilent 1100 module to module, 0.5m lg	5181-1516
Agilent 1100 module to module, 1m lg	5181-1519
Agilent 1100 module to control module	G1323-81600


External Contact Cable



One end of this cable provides a 15-pin plug to be connected to Agilent 1100 Series module's interface board. The other end is for general purpose.

Agilent 1100 Series Interface Board to general purposes

Connector G1103-61611	Color	Pin Agilent 1100	Signal Name
	White	1	EXT 1
	Brown	2	EXT 1
	Green	3	EXT 2
	Yellow	4	EXT 2
	Grey	5	EXT 3
	Pink	6	EXT 3
	Blue	7	EXT 4
	Red	8	EXT 4
	Black	9	Not connected
	Violet	10	Not connected
	Grey/pink	11	Not connected
	Red/blue	12	Not connected
	White/green	13	Not connected
	Brown/green	14	Not connected
	White/yellow	156	Not connected




RS-232 Cable Kit

This kit contains a 9-pin female to 9-pin female Null Modem (printer) cable and one adapter. Use the cable and adapter to connect Agilent Technologies instruments with 9-pin male RS-232 connectors to most PCs or printers.

Agilent 1100 module to PC

RS-232 Cable Kit [34398A](#)

Instrument

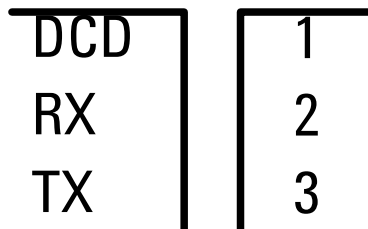

LAN Cables

Recommended Cables

For point to point connection (not using a network hub) use a twisted pair cross over LAN cable (P/N [5183-4649](#), 10 feet long).

For standard network connections using a hub use category 5 UTP cables, (P/N [G1530-61480](#), 8 m long).



6 Introduction to the Isocratic Pump

Introduction to the Isocratic Pump	190
Overview	191
How Does the Pump Work?	192
Electrical Connections	196
Instrument Layout	198
Early Maintenance Feedback (EMF)	199
The Electronics	201
The Low-Pressure Pump Main Board (LPM)	202
Firmware Description	206
Optional Interface Boards	208
Agilent 1100 Series Interfaces	211
Setting the 8-bit Configuration Switch	216
The Main Power Supply Assembly	221



Introduction to the Isocratic Pump

The isocratic pump comprises a pump assembly and a damping unit. Degassing is not included but a vacuum degasser is available as a separate product for applications that require best flow stability especially at low flow rates or highest detector sensitivity. This is most likely required to run small internal diameter columns (2 mm and 1 mm i.d.) which require low flow rates. A solvent cabinet provides enough space for up to four one liter bottles. A continuous seal wash (optional) is available when the pump is used with concentrated buffer solutions.

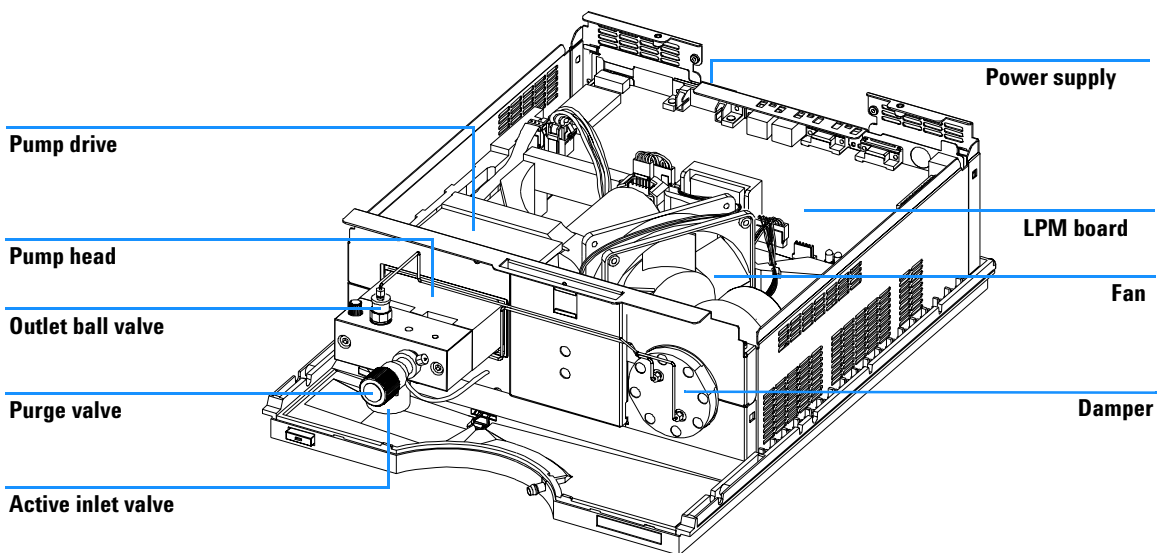


Figure 40 Overview of the Isocratic Pump

Overview

The isocratic pump is based on a two-channel, dual-plunger in-series design which comprises all essential functions that a solvent delivery system has to fulfill. Metering of solvent and delivery to the high-pressure side are performed by one pump assembly which can generate pressure up to 400 bar.

The pump assembly includes a pump head with an active inlet valve which has a replaceable cartridge, and an outlet valve. A damping unit is connected between the two plunger chambers. A purge valve including a PTFE frit is fitted at the pump outlet for convenient priming of the pump head.

A continuous seal wash (optional) is available when the isocratic pump is used with concentrated buffer solutions.

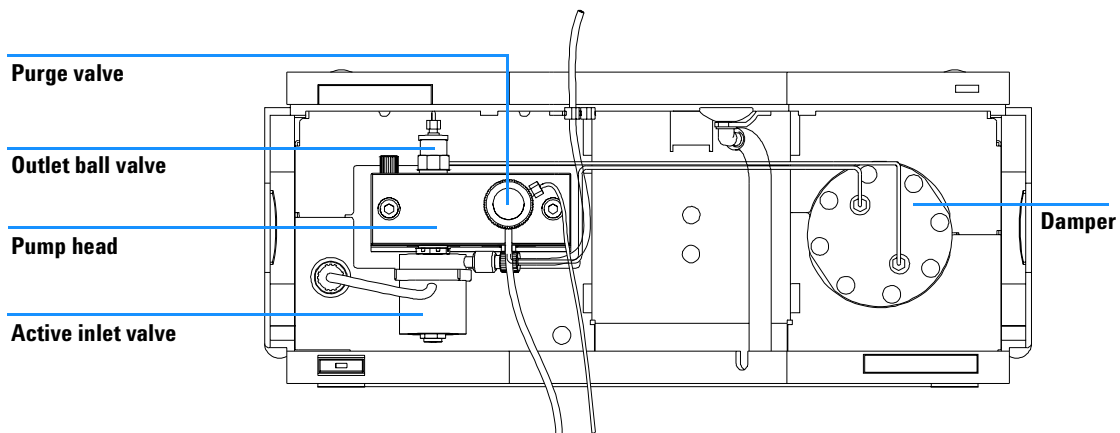


Figure 41 Hydraulic Path

How Does the Pump Work?

The liquid runs from the solvent reservoir to the active inlet valve. The pump assembly comprises two substantially identical plunger pump units. Both pump units comprise a ball-screw drive and a pump head with one sapphire plunger for reciprocating movement in it.

A servo-controlled variable reluctance motor drives the two ball screw drives in opposite directions. The gears for the ball-screw drives have different circumferences (ratio 2:1) allowing the first plunger to move at twice the speed of the second plunger. The solvent enters the pump heads close to the bottom limit and leaves it at its top. The outer diameter of the plunger is smaller than the inner diameter of the pump head chamber allowing the solvent to fill the gap in between. The first plunger has a stroke volume in the range of 20 – 100 μ l depending on the flow rate. The microprocessor controls all flow rates in a range of 1 μ l – 10 ml/min. The inlet of the first pumping unit is connected to the active inlet valve which is processor-controlled opened or closed allowing solvent to be drawn into the first plunger pump unit.

The outlet of the first plunger pump unit is connected through the outlet ball valve and the damping unit to the inlet of the second plunger pump unit. The outlet of the purge valve assembly is then connected to the following chromatographic system.

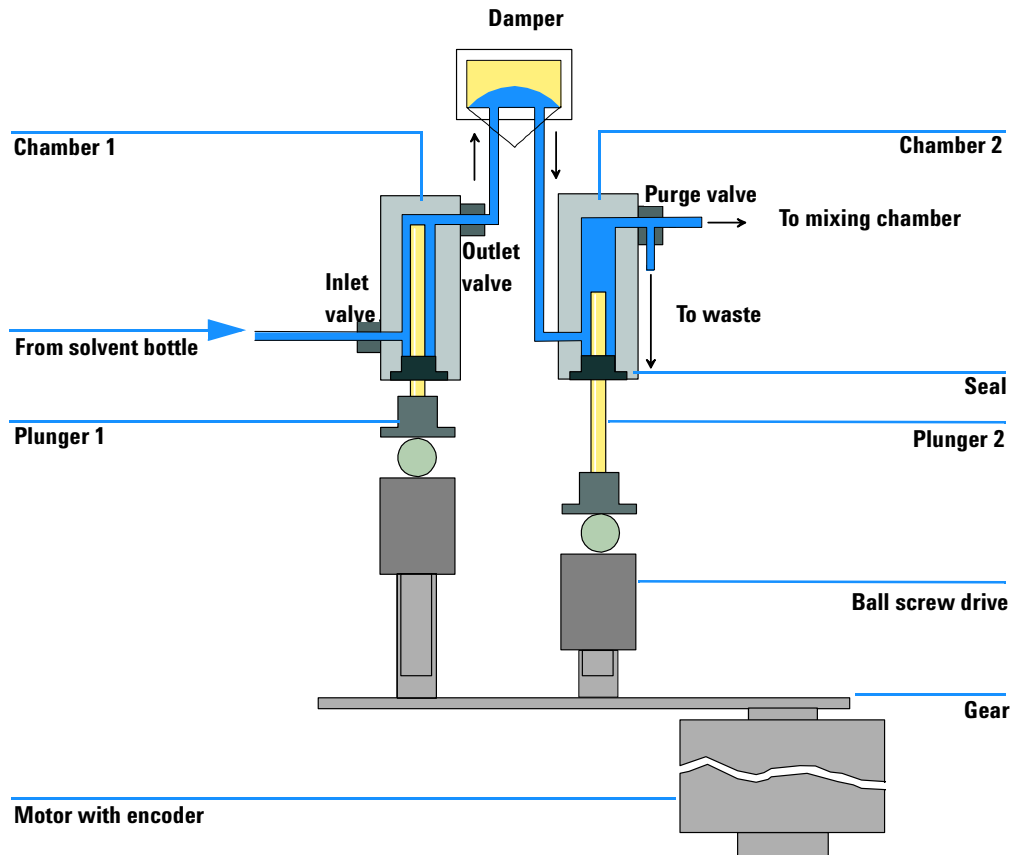


Figure 42 Principle of the Isocratic Pump

When turned on, the isocratic pump runs through an initialization procedure to determine the upper dead center of the first plunger. The first plunger moves slowly upwards into the mechanical stop of the pump head and from there it moves back a predetermined path length. The controller stores this plunger position in memory. After this initialization the isocratic pump starts operation with the set parameters. The active inlet valve is opened and the down-moving plunger draws solvent into the first pump head. At the same time the second plunger is moving upwards delivering into the system. After a controller-defined stroke length (depending on the flow rate) the drive motor is stopped and the active inlet valve is closed. The motor direction is reversed and moves the first plunger up until it reaches the stored upper limit and at

the same time moving the second plunger downwards. Then the sequence starts again moving the plungers up and down between the two limits. During the up movement of the first plunger the solvent in the pump head is pressed through the outlet ball valve into the second pumping unit. The second plunger draws in half of the volume displaced by the first plunger and the remaining half volume is directly delivered into the system. During the drawing stroke of the first plunger, the second plunger delivers the drawn volume into the system.

Table 26 Isocratic Pump Details

Delay volume	800–1100 μ l, dependent on back pressure
Materials in contact with mobile phase	
Pump head	SST, gold, sapphire, ceramic
Active inlet valve	SST, gold, sapphire, ruby, ceramic, PTFE
Outlet valve	SST, gold, sapphire, ruby
Adapter	SST, gold
Purge valve	SST, gold, PTFE, ceramic, PEEK

For pump specifications, see [Chapter 8](#), “Specifications.”

How Does Compressibility Compensation Work?

The compressibility of the solvents in use will affect retention-time stability when the back pressure in the system changes (for example, ageing of column). In order to minimize this effect, the pump provides a compressibility compensation feature which optimizes the flow stability according to the solvent type. The compressibility compensation is set to a default value and can be changed through the user interface.

Without a compressibility compensation the following will happen during a stroke of the first plunger. The pressure in the plunger chamber increases and the volume in the chamber will be compressed depending on backpressure and solvent type. The volume displaced into the system will be reduced by the compressed volume.

With a compressibility value set the processor calculates a compensation volume, that is depending on the backpressure in the system and the selected compressibility. This compensation volume will be added to the normal stroke volume and compensates the previous described *loss* of volume during the delivery stroke of the first plunger.

How Does Variable Stroke Volume Work?

Due to the compression of the pump-chamber volume each plunger stroke of the pump will generate a small pressure pulsation, influencing the flow ripple of the pump. The amplitude of the pressure pulsation is mainly dependent on the stroke volume and the compressibility compensation for the solvent in use. Small stroke volumes will generate pressure pulsations of smaller amplitude than higher stroke volumes at same flow rates. In addition the frequency of the pressure pulsations will be higher. This will decrease the influence of flow pulsations on quantitative results.

In gradient mode smaller stroke volumes resulting in less flow ripple will improve composition ripple.

The isocratic pump uses a processor-controlled spindle system to drive its plungers. The normal stroke volume is optimized for the selected flow rate. Small flow rates use a small stroke volume while higher flow rates use a higher stroke volume.

The stroke volume for the pump is set to AUTO mode. This means that the stroke is optimized for the flow rate in use. A change to larger stroke volumes is possible but not recommended.

Electrical Connections

- The GPIB connector is used to connect the pump with a computer. The address and control switch module next to the GPIB connector determines the GPIB address of your pump. The switches are preset to a default address ([Table 29](#) on page 211 or [Table 33](#) on page 216). This address is recognized at powercycling the module.
- The CAN bus is a serial bus with high speed data transfer. The two connectors for the CAN bus are used for internal Agilent 1100 Series module data transfer and synchronization.
- One analog output provides a pressure signal for integrators or data handling systems.
- The interface board slot is used for external contacts and BCD bottle number output or LAN connections.
- The REMOTE connector may be used in combination with other analytical instruments from Agilent Technologies if you want to use features such as start, stop, common shut down, prepare, and so on.
- With the appropriate software, the RS-232C connector may be used to control the module from a computer through a RS-232C connection. This connector is activated and can be configured with the configuration switch next to the GPIB connector (see [“Communication Settings for RS-232C Communication”](#) on page 218). See your software documentation for further information.
- The power input socket accepts a line voltage of 100–120 or 220–240 volts AC \pm 10% with a line frequency of 50 or 60 Hz. Maximum power consumption is 220 VA. There is no voltage selector on your module because the power supply has wide-ranging capability. There are no externally accessible fuses, because automatic electronic fuses are implemented in the power supply. The security lever at the power input socket prevents the module cover from being taken off when line power is still connected.

WARNING

Never use cables other than the ones supplied by Agilent Technologies to ensure proper functionality and compliance with safety or EMC regulations.

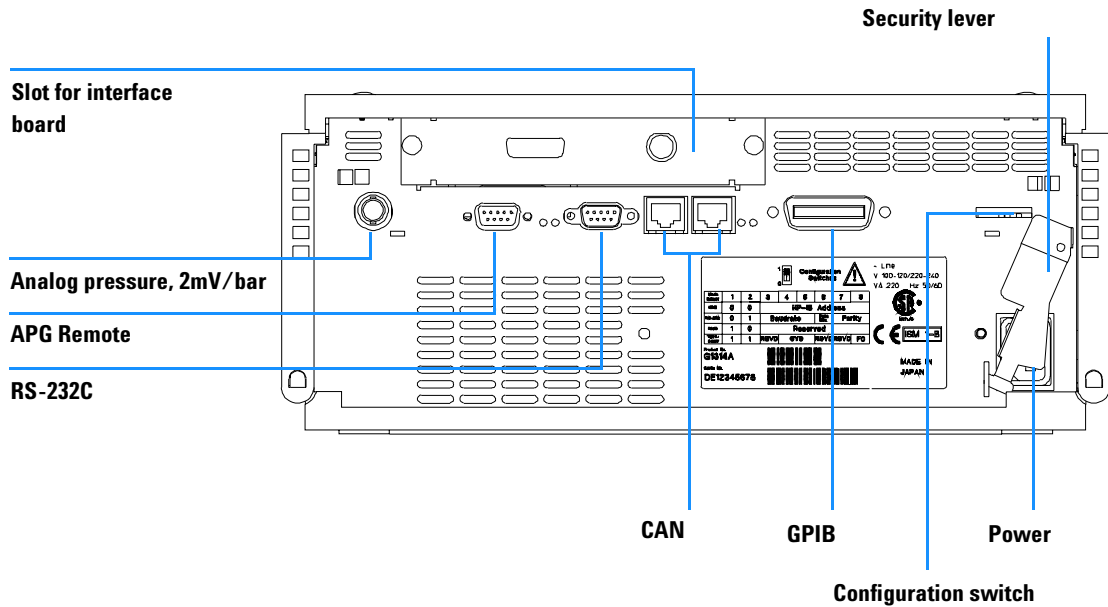


Figure 43 Electrical Connections

WARNING

To disconnect the isocratic pump from line, unplug the power cord. The power supply still uses some power, even if the power switch on the front panel is turned off.

Instrument Layout

The industrial design of the module incorporates several innovative features. It uses Agilent's E-PAC concept for the packaging of electronics and mechanical assemblies. This concept is based upon the use of expanded polypropylene (EPP) layers foam plastic spacers in which the mechanical and electronic boards components of the module are placed. This pack is then housed in a metal inner cabinet which is enclosed by a plastic external cabinet. The advantages of this packaging technology are:

- virtual elimination of fixing screws, bolts or ties, reducing the number of components and increasing the speed of assembly/disassembly,
- the plastic layers have air channels molded into them so that cooling air can be guided exactly to the required locations,
- the plastic layers help cushion the electronic and mechanical parts from physical shock, and
- the metal inner cabinet shields the internal electronics from electromagnetic interference and also helps to reduce or eliminate radio frequency emissions from the instrument itself.

Early Maintenance Feedback (EMF)

Maintenance requires the exchange of components in the flow path which are subject to mechanical wear or stress. Ideally, the frequency at which components are exchanged should be based on the intensity of usage of the instrument and the analytical conditions, and not on a predefined time interval. The early maintenance feedback (EMF) feature monitors the usage of specific components in the instrument, and provides feedback when the user-settable limits have been exceeded. The visual feedback in the user interface provides an indication that maintenance procedures should be scheduled.

EMF Counters

The isocratic pump provides a series of EMF counters for the pump head. Each counter increments with pump use, and can be assigned a maximum limit which provides visual feedback in the user interface when the limit is exceeded. Each counter can be reset to zero after maintenance has been done. The isocratic pump provides the following EMF counters:

- Pump Liquimeter
- Pump seal wear

Pump Liquimeter

The pump liquimeter displays the total volume of solvent pumped by the pump head since the last reset of the counters. The pump liquimeter can be assigned an EMF (maximum) limit. When the limit is exceeded, the EMF flag in the user interface is displayed.

Seal Wear Counters

The seal wear counters display a value derived from pressure and flow (both contribute to seal wear). The values increment with pump usage until the counters are reset after seal maintenance. Both seal wear counters can be assigned an EMF (maximum) limit. When the limit is exceeded, the EMF flag in the user interface is displayed.

Using the EMF Counters

The user-settable EMF limits for the EMF counters enable the early maintenance feedback to be adapted to specific user requirements. The wear of pump components is dependent on the analytical conditions, therefore, the definition of the maximum limits need to be determined based on the specific operating conditions of the instrument.

Setting the EMF Limits

The setting of the EMF limits must be optimized over one or two maintenance cycles. Initially, no EMF limit should be set. When performance indicates maintenance is necessary, take note of the values displayed by pump liquimeter and seal wear counters. Enter these values (or values slightly less than the displayed values) as EMF limits, and then reset the EMF counters to zero. The next time the EMF counters exceed the new EMF limits, the EMF flag will be displayed, providing a reminder that maintenance needs to be scheduled.

The Electronics

The electronics are comprised of four main components:

- **The low pressure pump main board (LPM)**, see [page 202](#).
- **Power supply**, see [page 221](#).

Optional:

- **Interface board (BCD/external contacts)**, see [page 208](#).
- **Interface board (LAN)**, see [page 209](#).

The Low-Pressure Pump Main Board (LPM)

The board controls all information and activities of all assemblies within the isocratic pump. The operator enters parameters, changes modes and controls the isocratic pump through interfaces (CAN, GPIB or RS-232C) connected to the user-interfaces. [Figure 45](#) on page 204 and [Figure 46](#) on page 205 show the block diagrams of this board.

ASIC — Application-Specific Integrated Circuit

The application-specific integrated circuit (ASIC) includes all digital logic for the core processor functions and also for module-specific functions.

Motor Drive

The drive comprises motor control, motor amplifier (drive) and current control.

Active Inlet Valve Drive

The drive comprises two amplifiers for the two contacts of valve solenoid.

Pressure Converter

This block comprises a filter and amplifier for the pressure-sensor-signal, a multiplexer, an A/D converter and an offset correction for the analog pressure output signal. The output voltage is 2 mV/bar.

Leak Converter

This block comprises a PTC for the leak identification and a NTC for the ambient temperature measurement. This assures that temperature changes are not identified as leak. A leak would cool down the PTC and its change in resistance results in a leak signal.

Fan Drive

The fan speed is controlled by the main processor depending on the internal heat distribution in the isocratic pump. The fan provides a PWM signal which is proportional to its speed. This fan status signal is used for diagnostics.

Electronic Fuses

The valve circuits are electronically fused on the board. Any error on the board or shortages of the valves will activate the electronic fuses that will switch off the supply voltage. This prevents the damage to components.

Onboard Battery

An onboard lithium battery buffers the electronic memories when the isocratic pump is turned off.

For safety information on Lithium batteries see "[Lithium Batteries Information](#)" on page 253.

Interfaces

The isocratic pump provides the following interfaces:

- two CAN connectors as interface to other Agilent 1100 Series modules
- one GPIB connector as interface to the ChemStation
- one RS-232C for as interface to a computer
- one REMOTE connector as interface to other Agilent products
- one Analog Output for pressure signal output
- one o
- ptional interface board

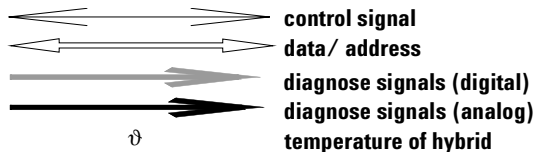


Figure 44 Block Diagram Signal Explanations

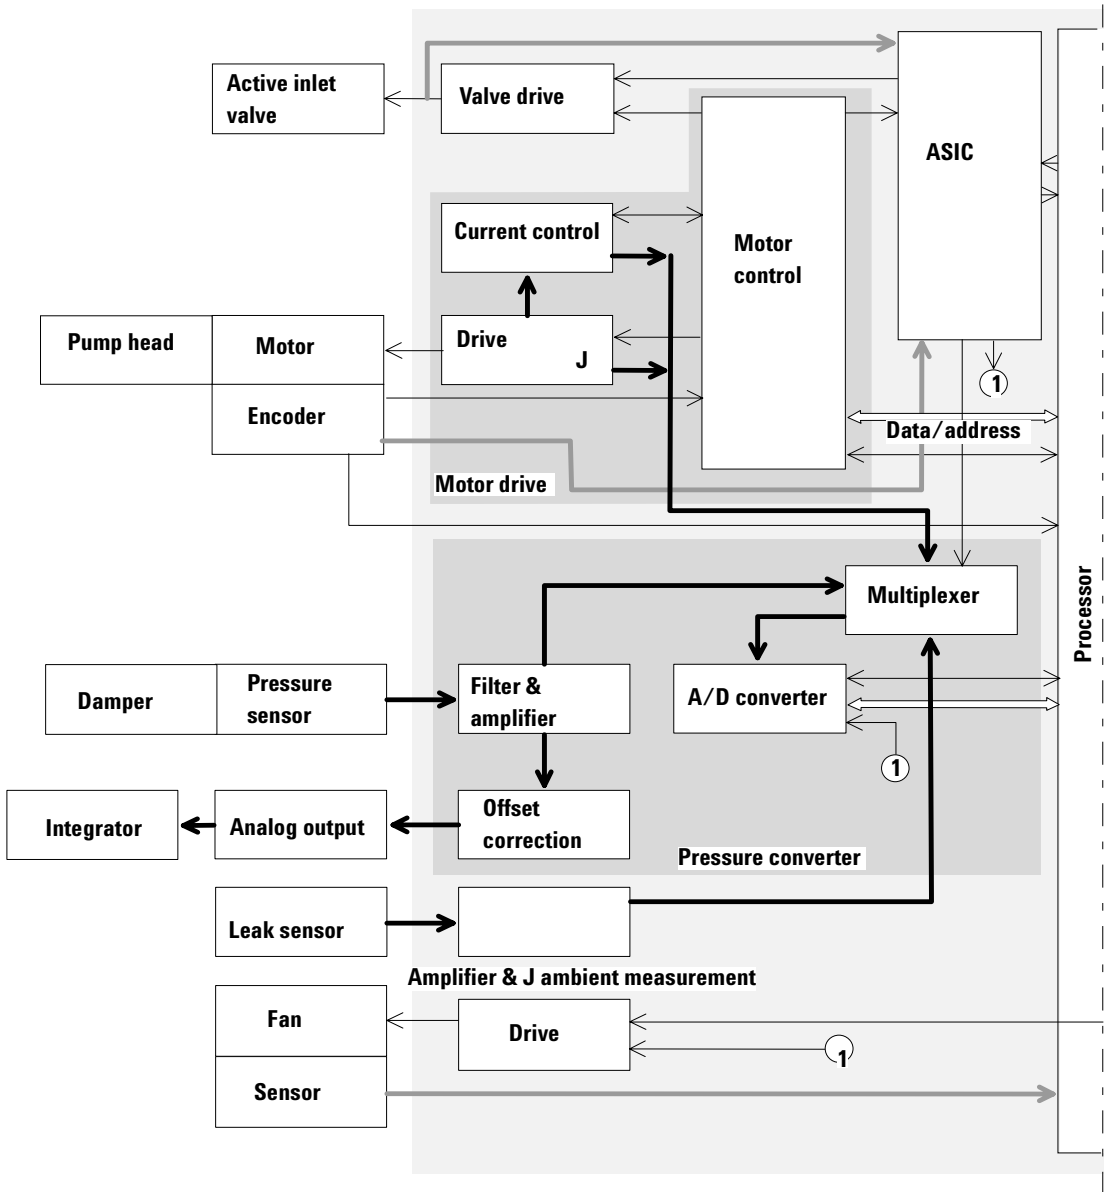


Figure 45 Block Diagram Pump Controller Board

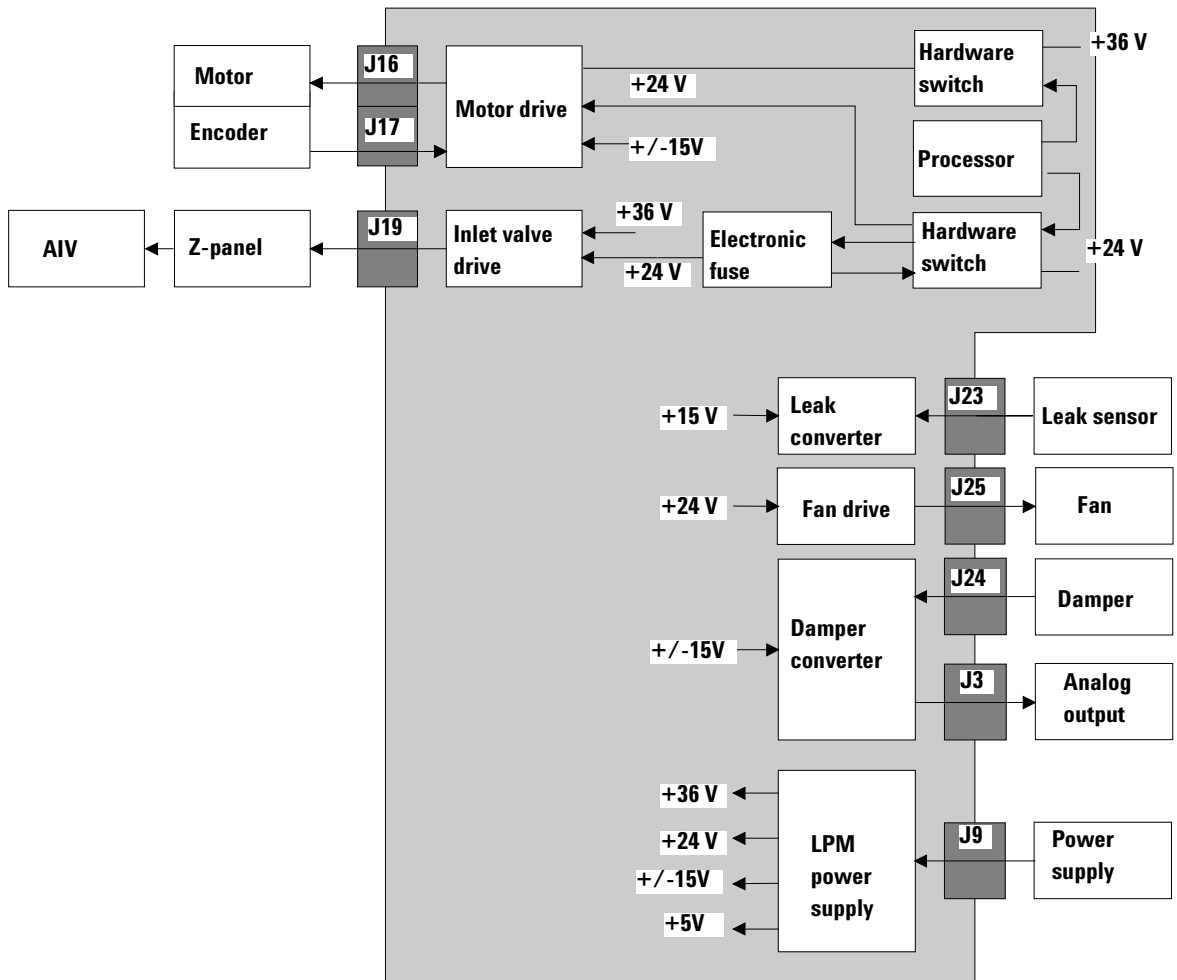


Figure 46 Interconnection Diagram Low Pressure Main Board (LPM)

Firmware Description

The firmware of the instrument consists of two independent sections:

- a non-instrument specific section, called 'resident system',
- an instrument specific section, called 'main system'.

Resident System

This resident section of the firmware is identical for all Agilent 1100 series modules. Its properties are:

- the complete communication capabilities (GPIB, CAN, LAN and RS-232C),
- memory management,
- ability to update the firmware of the 'main system'.

Main System

Its properties are:

- the complete communication capabilities (GPIB, CAN, LAN and RS-232C),
- memory management,
- ability to update the firmware of the 'resident system'.

In addition the main system comprises the instrument functions that are divided into common functions like

- run synchronisation via APG remote
- error handling,
- diagnostic functions and so on,

or module specific functions like

- internal events such as motor control, flow rates and so on,
- calculation of compensation values for variable strokes and pressures.

Firmware Updates

Firmware updates can be done using your user interface:

- handheld control module with files from a PC-card or
- Agilent ChemStation with files from floppy disk

The file naming conventions are:

xxxx-vvv.DLB, where

xxxx is the product number, e.g. 1310 for the G1310A isocratic Pump), and vvv is the revision number, for example 200 is revision 2.00.

For instructions refer to your user interface.

NOTE

Update of main system can be done in the resident system only.

Update of the resident system can be done in the main system only.

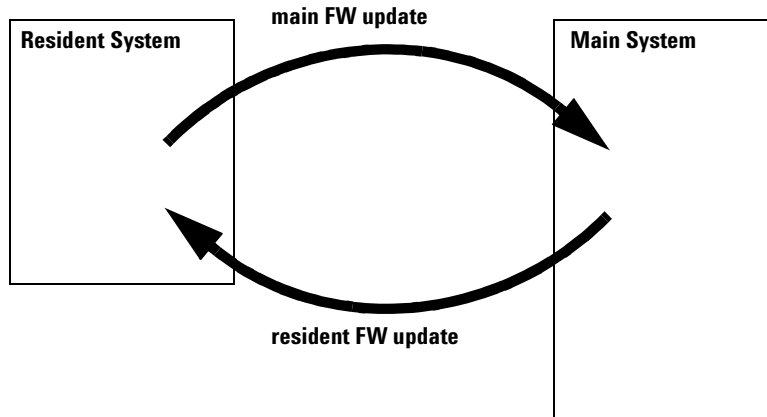


Figure 47 Firmware Update Mechanism

Optional Interface Boards

The Agilent 1100 Series modules have one optional board slot that allows to add an interface board to the modules.

Table 27 Optional Interface Boards

Description	Part Number
BCD Board	G1351-68701
Fuse 250 mA (four are on the board)	2110-0004
LAN Board (see next page for details)	

BCD Board

The BCD board provides a BCD output for the bottle number of the Agilent 1100 Series autosampler and four external contacts. The external contact closure contacts are relay contacts. . The maximum settings are: 30 V (AC/DC); 250 mA (fused). There are general purpose cables available to connect the BCD output, see “[BCD Cables](#)” on page 181 and the external outputs, see “[External Contact Cable](#)” on page 185 to external devices.

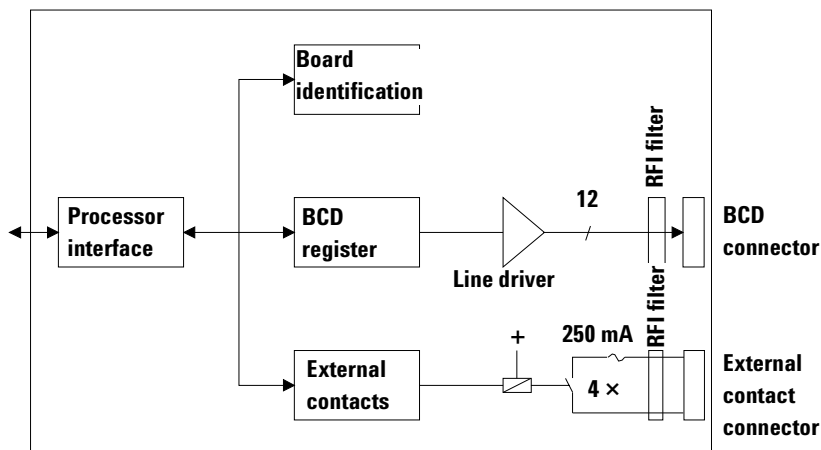


Figure 48 Block Diagram BCD Board

LAN Board

The HP LAN board is actually an HP JetDirect card, which is a network interface card used in HP printers.

NOTE

One board is required per Agilent 1100 stack. If the Agilent 1100 stack has a DAD, then the DAD **MUST** be the module used for LAN board installation. If no DAD is present a pump should be used for the LAN board installation.

NOTE

The LAN board can only be used together with:

A DAD/MWD/VWD/Pump/ALS with main board version G13XX-66520 and greater. An FLD/RID with main board version G13XX-66500 and greater.

a DOS-ChemStation software revision A.06.01 or above.

The following boards can be used with the Agilent 1100 modules.

Table 28 LAN Boards

Agilent Order Number	Supported networks
J4106A	Ethernet/802.3, RJ-45 (10Base-T)
J4105A	Token Ring/802.5, DB9, RJ-45 (10Base-T)
J4100A	Fast Ethernet, Ethernet/802.3, RJ-45 (10/100Base-TX) + BNC (10Base2)

NOTE

Minimum firmware of the LAN boards is A.05.05.

Recommended Cables

For point to point connection (not using a network hub) use a twisted pair cross over LAN cable (P/N 5183-4649, 10 feet long).

For standard network connections using a hub use category 5 UTP cables, (P/N G1530-61480, 8 m long).

Agilent 1100 Series Interfaces

The Agilent 1100 Series modules provide the following interfaces:

Table 29 Agilent 1100 Series Interfaces

Interface Type	Pumps	Autosampler	DA Detector MW Detector FL Detector	VW Detector RI Detector	Thermostatted Column Compartment	Vacuum Degasser
CAN	Yes	Yes	Yes	Yes	Yes	No
GPIB	Yes	Yes	Yes	Yes	Yes	No
RS-232C	Yes	Yes	Yes	Yes	Yes	No
APG Remote	Yes	Yes	Yes	Yes	Yes	Yes
Analog	Yes	No	2 ×	1 ×	No	Yes*
Interface board	Yes	Yes	Yes	Yes	No	No

* The vacuum degasser will have a special connector for specific use. For details, see the degasser manual.

- The CAN connectors serve as the interface between the Agilent 1100 Series modules themselves,
- the GPIB connector serves as the interface between an Agilent 1100 module and the Agilent ChemStation,
- RS-232C provides an interface to a computer,
- the APG remote connector serves as the interface between the Agilent 1100 and other Agilent (APG remote compatible) products,
- the analog output connector(s) provide an analog signal output,
- the interface board slot (not common to all modules) provides specific interfacing needs (external contacts, BCD, LAN and so on).

WARNING

Never use cables other than the ones supplied by Agilent Technologies to ensure proper functionality and compliance with safety or EMC regulations, see ["Cable Overview"](#) on page 171.

Analog Signal Output

The analog signal output can be distributed to a recording device. For details refer to the description of the main board of the module.

GPIB Interface

The GPIB connector is used to connect the module with a computer. The address and control switches next to the GPIB connector determine the GPIB address of your module. The switches are preset to a default address and recognized by the operating software from Agilent Technologies.

Table 30 Default GPIB Addresses

G131x Pumps	22	DAD (HP 1040)	15
G1313 Autosampler	28	FLD (HP 1046)	12
G1327 Thermostatted Sampler	28	ECD (HP 1049)	11
G1316 Column Compartment	27		
G1314 VWD	24	Pumps (HP 1050)	16
G1315/G1365 DAD/MWD	26	Autosampler (HP 1050)	18
G1321 FLD	23	VWD (HP 1050)	10
G1362 RID	29	DAD (HP 1050)	17
		MWD (HP 1050)	17
Agilent 8453A	25		

CAN Interface

The CAN is an inter module communication interface. It is a 2 wire serial bus system supporting high speed data communication and real-time requirements.

APG Remote Interface

The APG Remote connector may be used in combination with other analytical instruments from Agilent Technologies if you want to use features as common shut down, prepare, and so on.

Remote control allows easy connection between single instruments or systems to ensure coordinated analysis with simple coupling requirements.

The subminiature D connector is used. The isocratic pump provides one remote connector which is inputs/outputs (wired-or technique).

To provide maximum safety within a distributed analysis system, one line is dedicated to SHUT DOWN the system's critical parts in case any module detects a serious problem. To detect whether all participating modules are switched on or properly powered, one line is defined to summarize the POWER ON state of all connected modules. Control of analysis is maintained by signal readiness READY for next analysis, followed by START of run and optional STOP of run triggered on the respective lines. In addition PREPARE and START REQUEST may be issued. The signal level are defined as:

- standard TTL levels (low = 0.0 - 0.8 V, high = +2.0 - 5.0 V)
- fan-out is 10,
- input load is 1.7 kOhm against + 5 V, and
- output are open collector type, inputs/outputs (wired-or technique).

Table 31 APG Remote Signal Distribution

Pin	Signal	Description
1	DGND	Digital ground
2	PREPARE	(L) Request to prepare for analysis (for example, detector lamp on). Receiver is any module performing preanalysis activities.
3	START	(L) Request to start run / timetable. Receiver is any module performing run-time controlled activities.
4	SHUT DOWN	(L) System has serious problem (for example, leak: stops pump). Receiver is any module that needs to be shutdown to avoid a safety risk.
5		Not used

Table 31 APG Remote Signal Distribution (continued)

Pin	Signal	Description
6	POWER ON	(H) All modules connected to system are switched on. Receiver is any module relying on operation of others.
7	READY	(H) System is ready for next analysis. Receiver is any sequence controller.
8	STOP	(L) Request to reach system ready state as soon as possible (for example, stop run, abort or finish and stop injection). Receiver is any module performing run-time controlled activities.
9	START REQUEST	(L) Request to start injection cycle. Receiver is the autosampler.

RS-232C

The RS-232C connector is used to control the instrument from a computer through RS-232C connection, using the appropriate software. This connector can be configured with the configuration switch module next to the GPIB connector. The RS-232C is designed as DCE (data communication equipment) with a 9-pin male SUB-D type connector. The pins are defined as:

Table 32 RS-232C Connection Table

Pin	Direction	Function
1	In	DCD
2	In	RxD
3	Out	TxD
4	Out	DTR
5		Ground
6	In	DSR
7	Out	RTS
8	In	CTS
9	In	RI

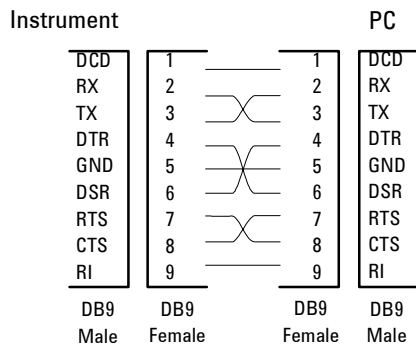


Figure 49 RS-232 Cable

Setting the 8-bit Configuration Switch

The 8-bit configuration switch is located next to the GPIB connector. Switch settings provide configuration parameters for GPIB address, serial communication protocol and instrument specific initialization procedures.

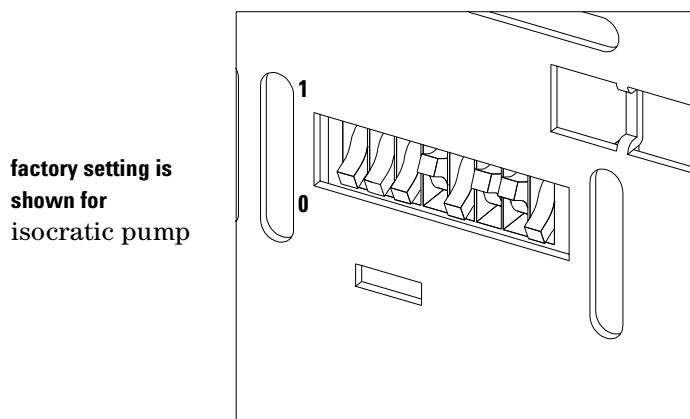


Figure 50 8-bit Configuration Switch

Table 33 8-bit Configuration Switch

Mode Select	1	2	3	4	5	6	7	8
GPIB	0	0		GPIB Address				
RS-232C	0	1	Baudrate			Data Bits	Parity	
Reserved	1	0	Reserved					
TEST/BOOT	1	1	RSVD	SYS		RSVD	RSVD	FC

Switches 1 and 2 define which set of parameters (for example, for GPIB, RS-232C, and so on) will be changed. Once the change has been completed, the instrument must be powered up again in order to store the values in the non-volatile memory.

In the non-volatile memory the parameters are kept, regardless of whether you turn the instrument off and on again. They will be kept until the same set of parameters is subsequently changed and power is reset. All other previously stored configuration settings will still remain in the non-volatile memory.

In this way you can store more than one set of parameters using the same 8-bit configuration switch twice,, for example, for both GPIB and RS-232C.

GPIB Default Addresses

If you just want to change the GPIB address and need a detailed procedure, refer to the *Installing Your ChemStation System* handbook. Default GPIB address is set to the following addresses::

Table 34 Default Addresses for Agilent Series 1100 Modules

Module	Address	Binary Address
Pump	22	00010110
FLD	12	00010111
VWD	24	00011000
Agilent 8453A	25	00011101
DAD/MWD	26	00011010
Column compartment	27	00011011
Autosampler	28	00011100
RID	29	00011101

where 0 means that the switch is down and 1 means that the switch is up.

Communication Settings for RS-232C Communication

The communication protocol used in the instrument supports only hardware handshake (CTS/RTR).

Switches 1 in down and 2 in up position define that the RS-232C parameters will be changed. Once the change has been completed, the instrument must be powered up again in order to store the values in the non-volatile memory.

Table 35 Communication Settings for RS-232C Communication

Mode Select	1	2	3	4	5	6	7	8
RS-232	0	1	Baudrate			Data Bits	Parity	

Use the following tables for selecting the setting which you want to use for RS-232C communication. The number 0 means that the switch is down and 1 means that the switch is up.

Table 36 Baudrate Settings

Switches			Baud Rate	Switches			Baud Rate
3	4	5		3	4	5	
0	0	0	9600 (default)	1	0	0	9600
0	0	1	1200	1	0	1	14400
0	1	0	2400	1	1	0	19200
0	1	1	4800	1	1	1	38400

Table 37 Data Bit Settings

Switch 6	Data Word Size
0	7 Bit Communication
1	8 Bit Communication

One start bit and one stop bit are always used (not selectable).

Per default, the module will turn into 19200 baud, 8 data bit with no parity.

Table 38 Parity Settings

Switches		Parity
7	8	
0	0	No Parity
0	1	Odd Parity
1	0	Even Parity

Forced Cold-Start Settings

Switches 1 and 2 do not force storage of this set of parameters in non-volatile memory. Returning the switches 1 and 2 to other positions (other than being both up) will allow for normal operation.

CAUTION

A forced cold start erases all methods and data stored in non-volatile memory. Exceptions are diagnose and repair logbooks will not be erased.

If you use the following switch settings and power the instrument up again, a forced cold start has been completed.

Table 39 Forced Cold Start Settings

Mode Select	1	2	3	4	5	6	7	8
TEST/BOOT	1	1	0	0	0	0	0	1

To return to normal operation, set switches back to your GPIB or RS 232C configuration settings.

Stay Resident Settings

Firmware update procedures may require this mode in case of firmware loading errors.

Switches 1 and 2 do not force storage of this set of parameters in non-volatile memory. Returning the switches 1 and 2 to other positions (other than being both up) will allow for normal operation.

If you use the following switch settings and power the instrument up again, the instrument firmware stays in the resident part, that is, it is not operable as an isocratic pump. It only uses basic functions of the operating system, for example, for communication, and so on.

Table 40 Stay Resident Settings

Mode Select	1	2	3	4	5	6	7	8
TEST/BOOT	1	1	0	0	1	0	0	0

To return to normal operation, set switches back to your GPIB or RS 232C configuration settings.

The Main Power Supply Assembly

The main power supply comprises a closed assembly (no component-level repair possibility).

The power supply provides all DC voltages used in the isocratic pump. The line voltage can vary in a range from 100 – 120 or 220 – 240 volts AC \pm 10 % and needs no manual setting.

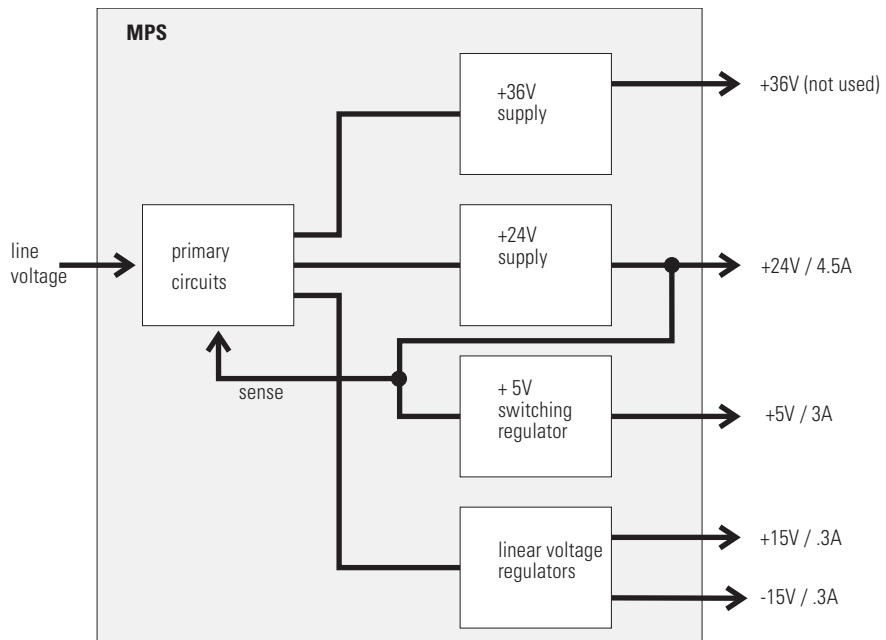


Figure 51 Main Power Supply (MPS) Block Diagram

WARNING

To disconnect the instrument from line, unplug the power cord. The power supply still uses some power, even if the power switch on the front panel is turned off.


No accessible hardware fuse is needed because the main power supply is safe against any short circuits or overload conditions on the output lines. When overload conditions occur, the power supply turns off all output voltages. Turning the line power off and on again resets the power supply to normal operation if the cause of the overload condition has been removed.

An over-temperature sensor in the main power supply is used to turn off output voltages if the temperature exceeds the acceptable limit (for example, if the cooling fan of the isocratic pump fails). To reset the main power supply to normal operating conditions, turn the isocratic pump off, wait until it is approximately at ambient temperature and turn the isocratic pump on again.

The following table gives the specifications of the main power supply.

Table 41 Main Power Supply Specifications

Maximum power	130 W	Continuous output
Line Input	100 – 120 or 220 – 240 volts AC ± 10 %, line frequency of 50/60 Hz	Wide ranging
Output 1	+ 24 V / 4.5 A (maximum)	Total power consumption of +24V and
Output 2	+ 36 V / 2.5 A (maximum)	+36V must not exceed 107 W
Output 3	+ 5 V / 3 A	
Output 4	+ 15 V / 0.3 A	
Output 5	- 15 V / 0.3 A	

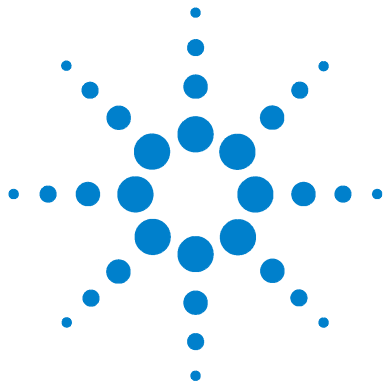

7 Control Module Screens for the Isocratic Pump

Major keys on the Agilent 1100 Control Module	224
Screens available from the Analysis screen	225
Screens available from the System screen	234
Screens available from the Records screen	236
Diagnostics and Tests	243



Major keys on the Agilent 1100 Control Module

Table 42

ESC	Return to previous screen and scroll through top layer views (Analysis, Settings)
m	Open context sensitive menus
i	Information/help
Enter	Store changed parameters or execute the choice from a pull-down menu
Done	(If available) Activate settings of current screen
On/Off	Switch on pump
Start	Start a run
Plot	View the pressure readings
Views	Change between view of analysis - status - system screens

NOTE

The screens shown on the next pages are based on the following firmware revisions:
Control Module firmware revision B.01.01 (G1323B).
LC Module firmware revision 3.8x


NOTE

In case the control module's display seems to be frozen (hang-up due to a communication problem on the CAN bus, unplug the control module from the LC module and reconnect.


Screens available from the Analysis screen

The Analysis screen

This is the wake-up screen, if the Agilent 1100 isocratic pump is the only configured Agilent 1100 module. It is used to enter the most common pump method parameters.

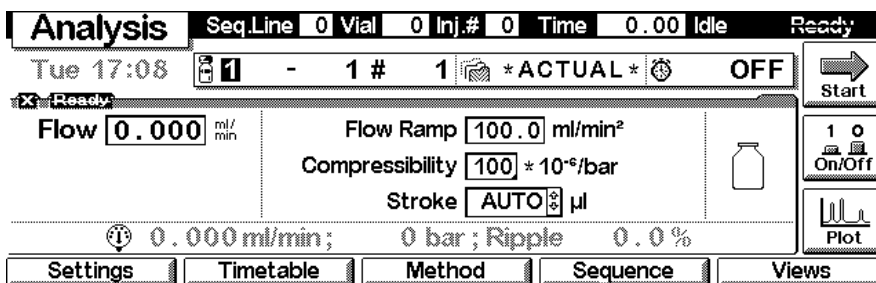


The **m**-key allows access to the context sensitive menu. **Date&Time** allows you to change time settings. **Print Screen** gives access to the print configuration screen. **About** tells you the current firmware revision and the serial# of your control module. **Setup view** leads you to add sections for additional Agilent 1100 modules. **Restart** re-boots the control module.

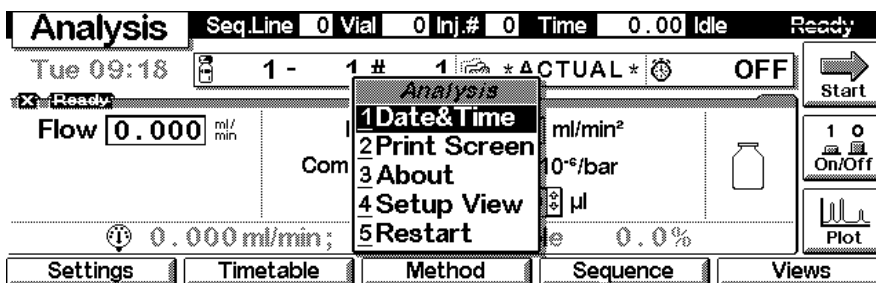


Setup View

In the Setup view, modules can be added or removed to the view.


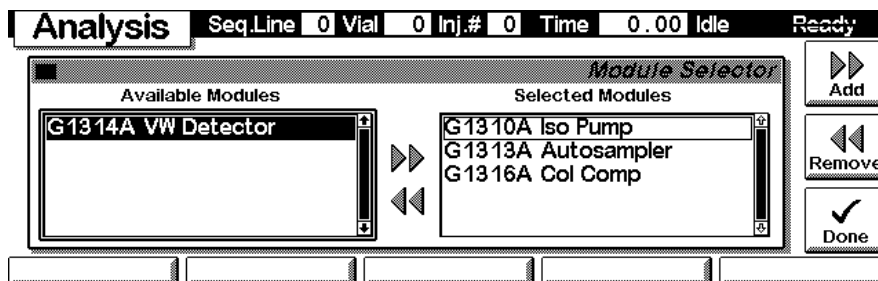


Here, e.g. the autosampler and thermostatted column compartment parameters are shown on the display as well. The number of parameters on the display is restricted as additional modules are added. A maximum of 4 modules is shown automatically. If more modules are connected to the system, you have to choose 4 of them in Setup view.

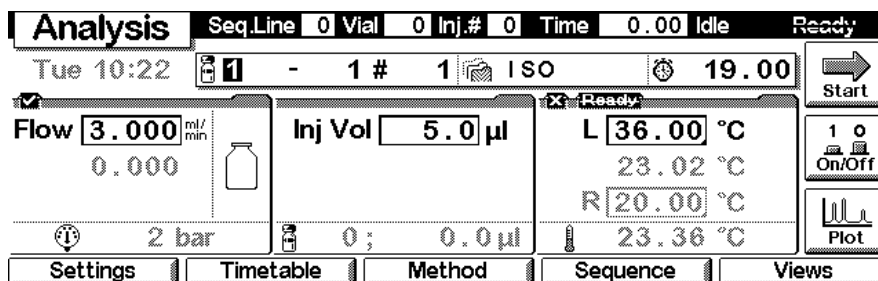


Pump ON/OFF

From the Analysis screen use the F7 key to proceed to the turn on screen. Press F8 (On) once to turn on the pump. If more than one module is available, select the isocratic pump from the pop-up menu.

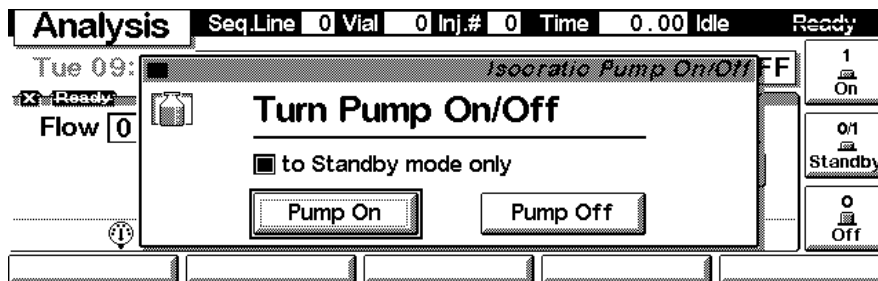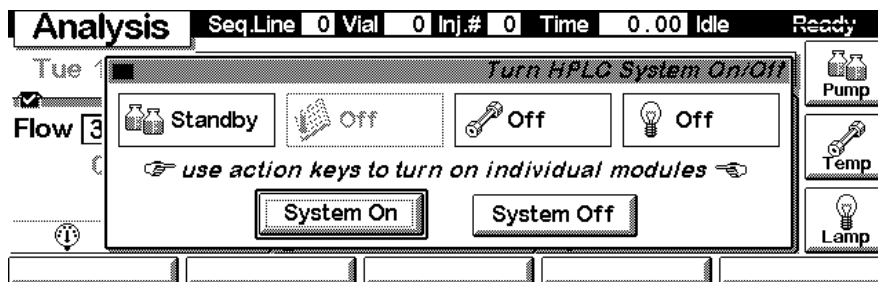

Settings


With the **Settings** key you open a pull-down menu where you can select the isocratic pump module.

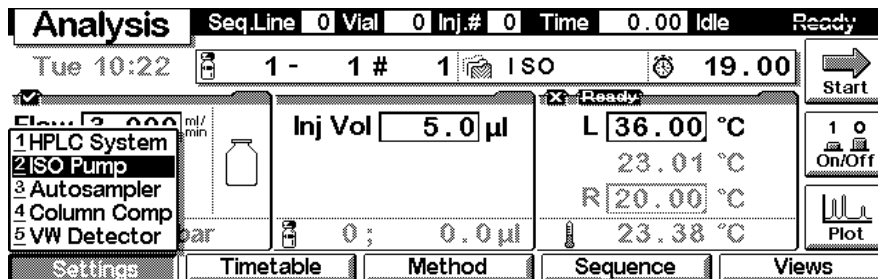


7 Control Module Screens for the Isocratic Pump

Settings

Within the **Settings** you can change the pump parameters. You have access to a different set of parameters available through the F1-5 keys. F7 key resets the pump to default values. F8 opens a window to turn on the pump.

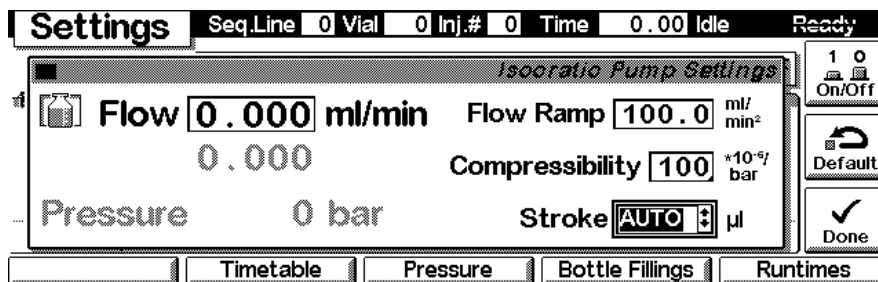

Use the **m**-key for the context sensitive menu. The **Status** command pulls up a monitor screen displaying signals and spectra as programmed. **Reset** will load the pump default parameters.

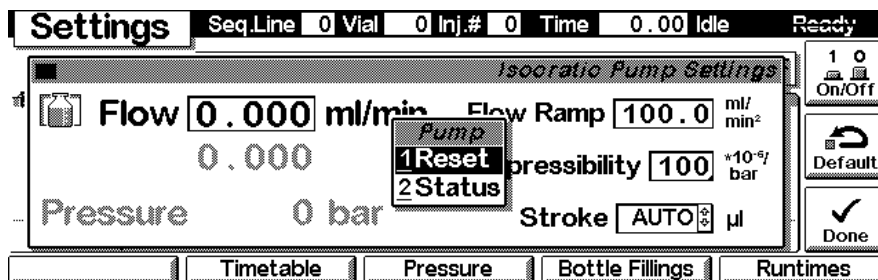

Settings - Timetable

With the F2 key (**Timetable**) you can list the timetable for the pump. Press F7 key (**Insert**) to add entries or F6 key (**Delete**) to remove entries.

Timetable				Seq.Line	0	Vial	0	Inj.#	0	Time	0.00	Idle	Ready
Time	Module	Setting	Value										
0.00	Iso Pump	Flow	1.000 ml/min										
5.00	Iso Pump	Flow	0.000 ml/min										
*** end of module timetable ***													

Insert
Delete

Use the F6 key (**Done**) to view the entered lines of the timetable.

Timetable				Seq.Line	0	Vial	0	Inj.#	0	Time	0.00	Idle	Ready
<i>Timetable Insert</i>													
Time [min]	Module	Setting											
0.00	Iso Pump	Flow											
			Flow 1.000 ml/min										
<i>fields change with setting selected</i>													

Enter
Done

Use the **m**-key for the context sensitive menu. It gives you additional tools for the timetable.

Timetable				Seq.Line	0	Vial	0	Inj.#	0	Time	0.00	Idle	Ready *
Time	Module	Setting	Value										
0.00	Iso Pump	Flow	1.000 ml/min										
5.00	Iso Pump	Flow	0.000 ml/min										
*** end of module timetable ***													

Timetable
1 Copy Line
2 Paste Line
3 Print Timetable
Insert
Delete

7 Control Module Screens for the Isocratic Pump

Settings - Pressure

With the F3 key (**Pressure**) you can change the settings for the pressure limits.

The screenshot shows the 'Settings' screen with the following data: Seq.Line 0, Vial 0, Inj.# 0, Time 0.00, Idle, Ready *. The main display area is titled 'Isocratic Pump Settings' and shows 'Pressure Limits' with 'Lower' set to 0 bar and 'Upper' set to 400 bar. The 'Actual Pressure' is 0 bar. On the right side, there are three buttons: a top button with a pressure gauge icon, a middle button with a checkmark icon, and a bottom button labeled 'Done' with a checkmark icon. The units on the right are ml/min², $\times 10^{-6}$ bar, and μ l.


Settings - Bottle Fillings

With the F4 key (**Bottle Fillings**) you can adjust the setting for the bottle filling to its current state.

The screenshot shows the 'Settings' screen with the following data: Seq.Line 0, Vial 0, Inj.# 0, Time 0.00, Idle, Ready *. The main display area is titled 'Isocratic Pump Settings' and shows 'Actual' and 'Total' both set to 0.00 Liter. At the bottom, there are two checkboxes: 'Not-Ready below' (checked) and 'Error if empty' (unchecked). On the right side, there are three buttons: a top button with a bottle icon and labeled 'Refill', a middle button with a checkmark icon, and a bottom button labeled 'Done' with a checkmark icon. The units on the right are ml/min², $\times 10^{-6}$ bar, and μ l.


Settings - Runtimes

With the F5 key (**Runtimes**) you can change the stop time and the post-run time.

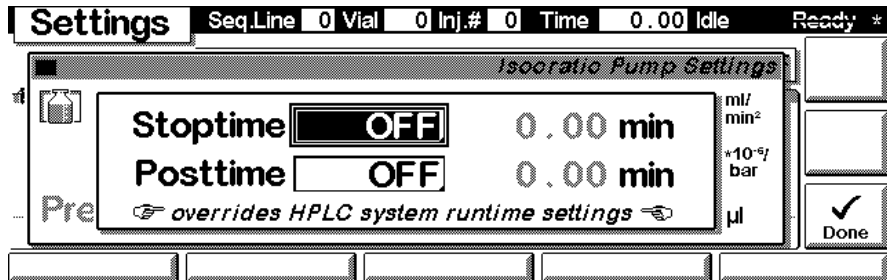


Analog - Status

Press F5 key (**Views**) and select **Status**.

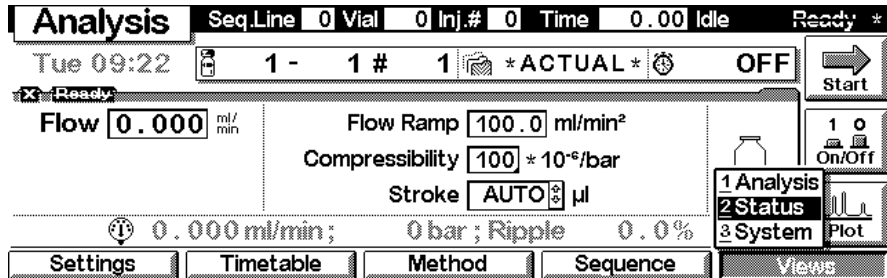


Status

This is an example if an Agilent 1100 pump is configured standalone. Information on the actual flow rate , pressure and %-ripple, elapsed run time and the pressure plot are shown. Press key F8 (**Start**) to start a run, key F7 (**Rescale**) to maximize the signal.

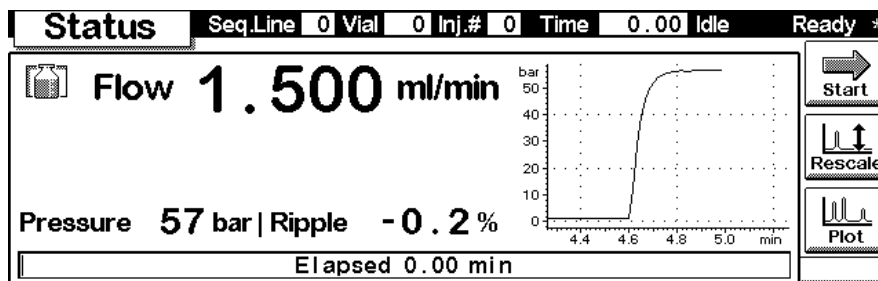


Signal plot

Press F6 key (**Plot**) to enter the plot screen (available also from the **Analysis** and **System** screen). Here you can observe the online signal(s). To add additional online signals (maximum 3), press F6 key (**Select**). If more than one signal is configured, use the 1-2-3 numeric keys to switch between the signals.

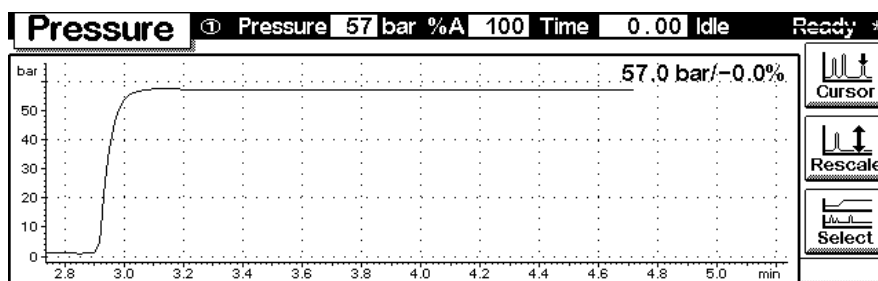


Press F6 key (**Select**). Here you can add additional online signals (maximum are 3). Additional signals could also be chromatograms or temperature signals from other modules. Use the Right/Left arrows to switch between Available and Selected Signals. Use the F8 key (**Move**) to enter available signals into the box for selected signals or vice versa. Press **Done** to activate the changed settings and to return to the **Plot** screen.

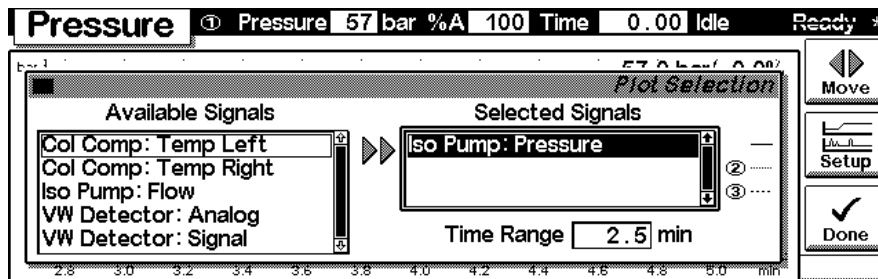


Method screens

On the **Analysis** screen use the F3 key (**Method**) to view the parameters in a method and F8 key (**Save As**) to save the method in the module(s). The PC-Card key is only active when a PCMCIA card is inserted in the control module (has to be inserted even before powercycling).

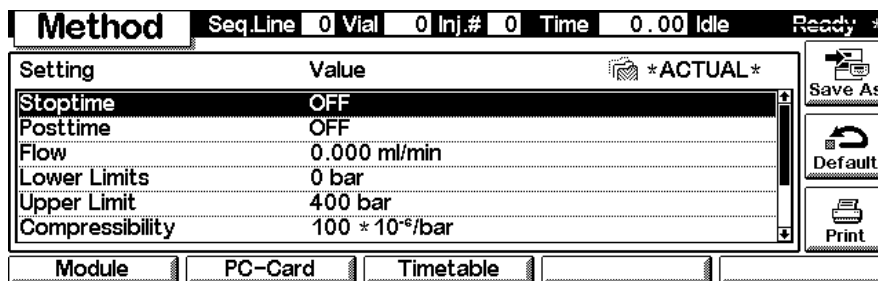

Use F2 key (**PC-Card**) to save a method on a PCMCIA card. Use the Right/Left arrows to switch between PC-Card and Instrument window. Use the UP/Down arrows to select the method. Use the F7/F8 keys (**Copy**) to enter available signals into the box for selected signals or vice versa.

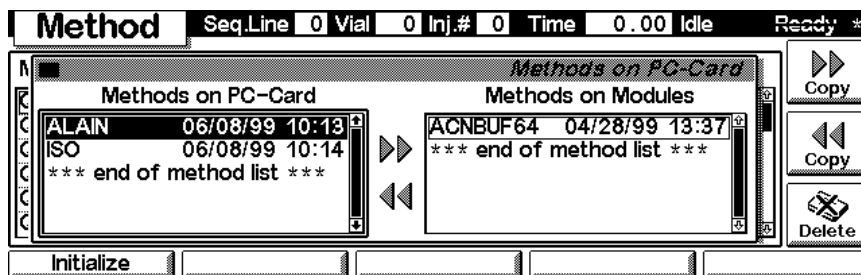

Screens available from the System screen

System screen

Use the Esc key to receive **Views** on the F5 key. Choose **System** from the pull-down menu. This screen shows the last activities in the system.

The screenshot shows the 'System' screen with the following elements:

- Header: **System** Pump Temp Lamp Time 0.00 Idle Ready *
- Status bar: Tue 10:26 TEMP OFF,LAMP OFF EMF Start
- Activity Log Table:

Module	Message	Id	Date	Time
Iso Pump	Setpoint changed	INFO	08/17	10:23:27
Iso Pump	Pump on	STATE	08/17	10:23:19
Iso Pump	Pump standby	STATE	08/17	10:22:13
Iso Pump	Init	STATE	08/17	10:21:45
Col Comp	Calibration done	STATE	08/17	10:20:43

Navigation buttons: Control, Configure, Tests, Records, Views

System - Control

Use the F1 key (**Control**) to select the isocratic pump. Here you receive information about the not-ready conditions if needed. F2 key (**Reset**) does a re-initialization of the pump.

The screenshot shows the 'System - Control' screen with the following elements:

- Header: **System** Pump Temp Lamp Time 0.00 Idle Ready *
- Status bar: Tue 10:26 TEMP OFF,LAMP OFF EMF Start
- Activity Log Table:

Module	Message	Id	Date	Time
1 HPLC System	Setpoint changed	INFO	08/17	10:23:27
2 ISO Pump	Pump on	STATE	08/17	10:23:19
3 Autosampler	Pump standby	STATE	08/17	10:22:13
4 Column Comp	Init	STATE	08/17	10:21:45
5 VW Detector	Calibration done	STATE	08/17	10:20:43

Navigation buttons: Control, Configure, Tests, Records, Views

System - Configuration

On the **System** screen use the F2 key (**Configure**) to select the pump. Use the F1 key (**Interfaces**) to access the interface settings (if required).

Config Pump Time 0.00 Idle Ready *

Isocratic Pump Configuration

Options

- 1 HP/IB
- 2 Serial
- 3 MIO
- 4 BCD Output

Interfaces Bottle Fillings

Done

Press F4 (**Bottle fillings**) to adjust bottle fillings to the current state.

Settings Seq.Line 0 Vial 0 Inj.# 0 Time 0.00 Idle Ready *

Isocratic Pump Settings

Actual 0.00 Liter ml/min²

Total 0.00 Liter *10⁻⁵/bar

Pre Not-Ready below 0.10 Liter Error if empty µl

Refill

Done

Screens available from the Records screen

Records screen

Use the Esc key to receive **Views** on the F5 key. Choose **System** from the pull-down menu. Use the F4 key (**Records**) to select the pump. Errors are reported either into the **System Log** (F2) or **Error Log** (F3).

Records						Pump <input checked="" type="checkbox"/>	Temp <input type="checkbox"/>	Lamp <input type="checkbox"/>	Time 0.00	Idle	Ready *
Module	Product#	Serial#	Version	On-Time	EMF						
Controller	G1323A*	DE53303495	A.02.02	0d 00:06h							
iso Pump	G1310A	US70601677	A.03.81	0d 00:07h							
Autosampler	G1313A	DE54800200	A.03.80	0d 00:18h							
Col Comp	G1316A*	US54300101	A.03.80	0d 00:18h							
VW Detector	G1314A	JP73704465	A.03.80	0d 00:18h							

Buttons: EMF, System Log, Error Log, Maint Log, FW Update

Icons: Identify, Print

System / Error Log

Use the F2 key (**System Log**) or F3 key (**Error Log**) to look for errors.

Records			Pump <input type="checkbox"/>	Time 0.00	Idle	Ready *
<i>isocratic Pump Error Logbook</i>						
Message	Date	Time				
Leak detected	08/16/99	11:13:36				
Compensation sensor short	08/16/99	11:13:36				
Pump configuration	08/16/99	11:11:29				
*** end of logbook ***						

Buttons: (empty)

Icon: Print


Info Log

Use the **m**-key to receive a pop-up menu, Select **Info Log**. A list of the last events are listed. For troubleshooting reasons they can be printed or saved to a file on the PCMCIA card (using the **m**-key for the context sensitive menu).


Records		Pump <input type="checkbox"/>	Time 0.00 Idle	Ready *
<i>Isocratic Pump Info Logbook</i>				
Message	Date	Time		
Info 1(0x00d9,36477)	08/17/99	07:45:56		
Info 1(0x00d9,10)	08/16/99	17:09:31		
Info (0x00d6,10)	08/16/99	17:03:21		
Info 1(0x00d9,10)	08/16/99	11:14:28		
On-Error action executed	08/16/99	11:11:29		
				Print

EMF (Early Maintenance Feedback)

Use the F1 key (**EMF**) to set EMF parameters. Choose menu item 1 (**Setup limits**) to select the amount of pumped solvent or seal wear, when you want to receive a warning for exceeded limits. Press F7 (**Reset**) to reset the counters after exchanging parts that are subject to wear.


Records		Pump <input type="checkbox"/>	Time 0.00 Idle	Ready *
<i>Isocratic Pump EMF Limits</i>				
 G1310A Iso Pump			Serial# US70601677	
Solvent pumped	0.00	Limit	<input type="text" value="OFF"/>	
Seal Wear	0	Limit	<input type="text" value="OFF"/>	
				Reset
				Done

If a set limit has been exceeded, a message box will pop up. This will not stop a sequence or run (information only to plan maintenance activities). If you press **Reset**, the limits will be removed. **Ignore** will continue to keep the EMF flag set.

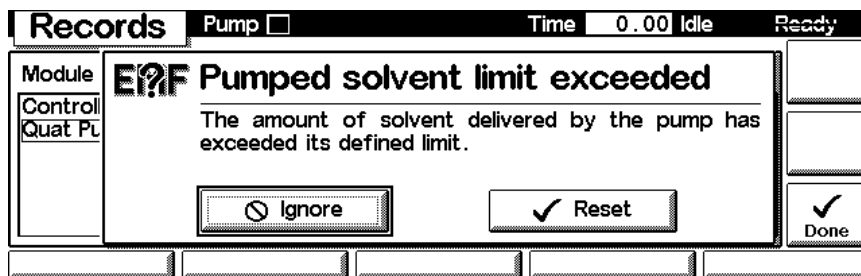


Firmware Update


Use the Esc key to receive **Views** on the F5 key. Choose **System** from the pull-down menu. Use the F3 key (**Records**) to select the pump. Use the F5 key (**FW Update**) to enter the Update section. If you want to update the resident firmware (together with specific main firmware revisions), select the file from the PCMCIA card (RESnnnn.DLB) and press execute. If you want to update the main firmware, press F7 key (**Transfer**) to turn the module into the resident mode (LED on module should blink yellow).

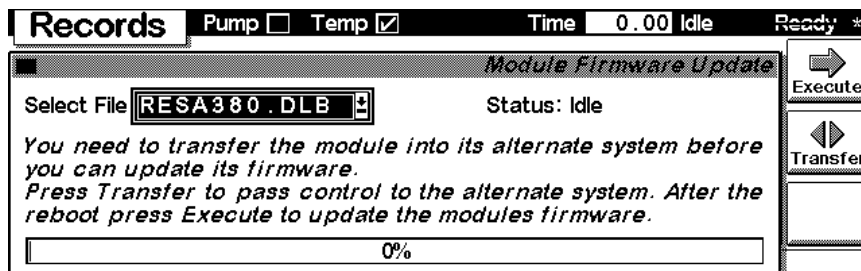


Use the **Esc** key to receive **Views** on the F5 key. Choose **System** from the pull-down menu. Use the F3 key (**Records**) to select the **Generic** module. In this screen the resident firmware revision is shown.

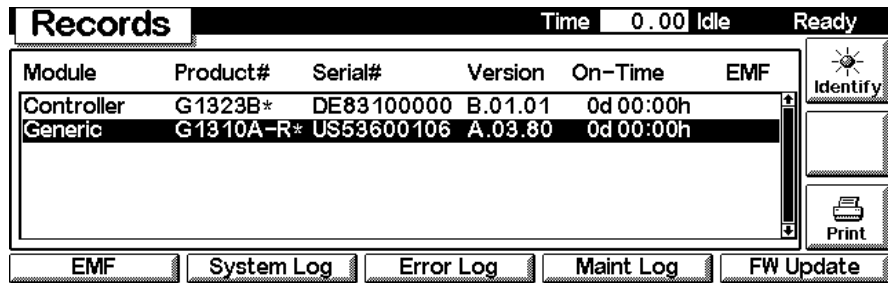

Use the F5 key (**FW Update**) to enter the Update section. Select the a file from the PCMCIA card (1310nnnn.DLB) and press execute. When the update has finished, press F7 key (**Transfer**) to return the module into the normal mode (LED on module should stay yellow).

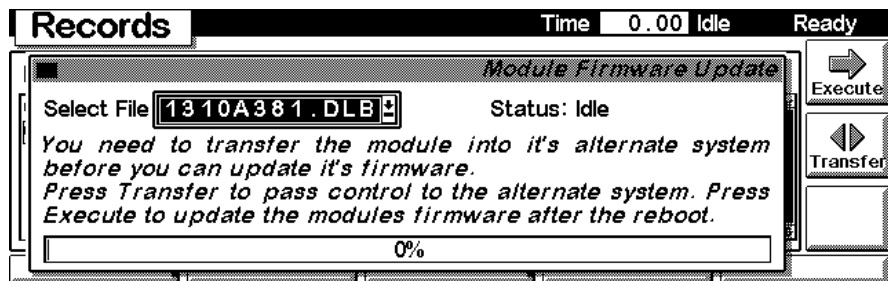



If you have not saved your methods, please do it before continuing. Otherwise they will be overwritten during the update process.

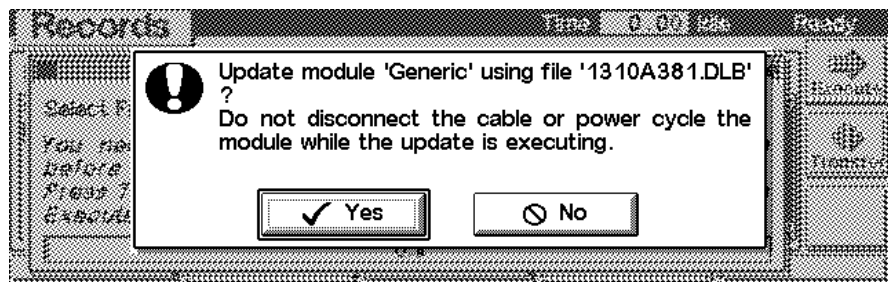

7 Control Module Screens for the Isocratic Pump


Changing the serial number

In case the serial number of the module has to be added, use the **m**-key to open the menu **Enter Serial#**. The serial number becomes active after restart of the module.

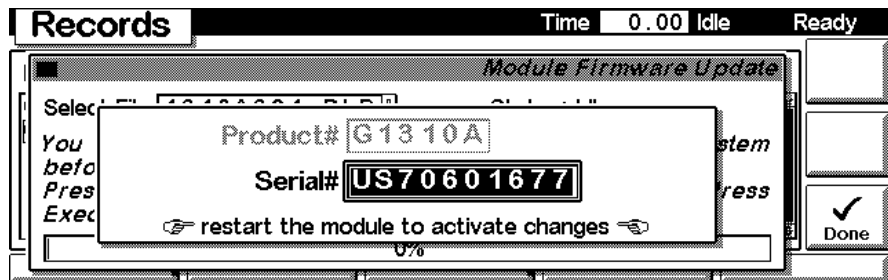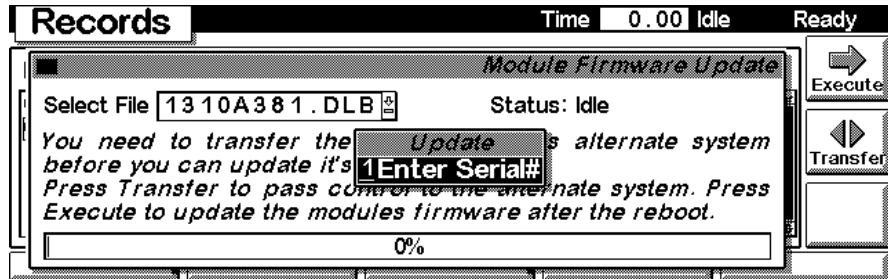


Maintenance activities

On the Records screen use the F4 key (**Maint log**) to view and edit the maintenance logbook.

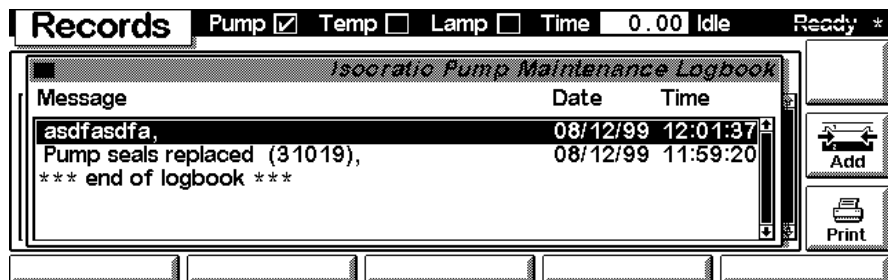


Use the F7 key (**Add**) to add new maintenance activities. If an activity is not listed, you can type the activity into the line “Add” using the control modules key pad.

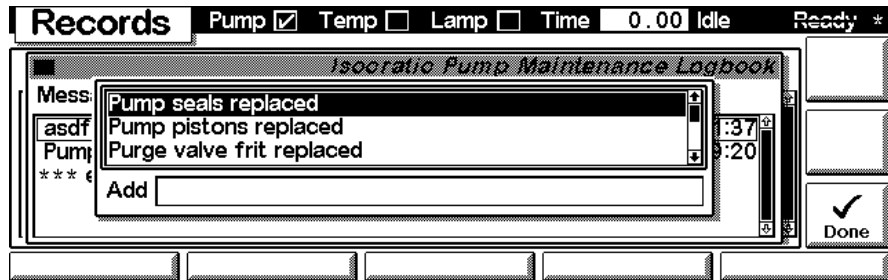


Changing the Type

In order to change the type of the module (this may be necessary after an exchange of the mainbord) press 'm.m' in the **Test**-screen and select **Command**.

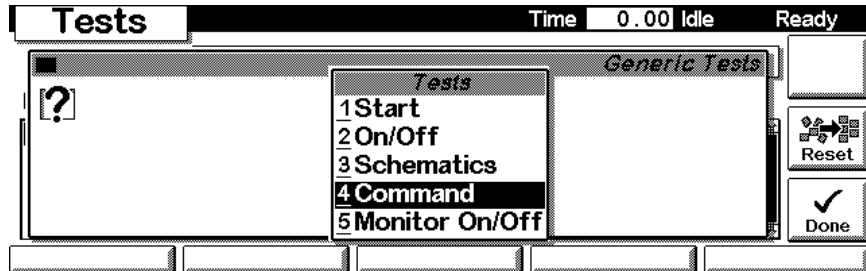


Enter 'TYPE G1310A' in the Instr-line in order to configure the module as a isocratic pump.

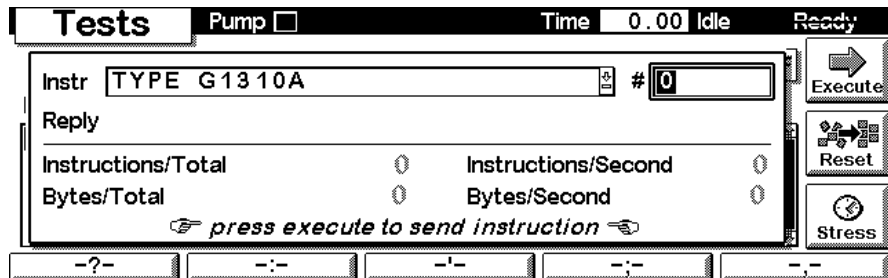

7 Control Module Screens for the Isocratic Pump

Schematics


Select **Schematics** after pressing 'm.m' on the Test-screen in order to get a schematic overview of the isocratic pump.

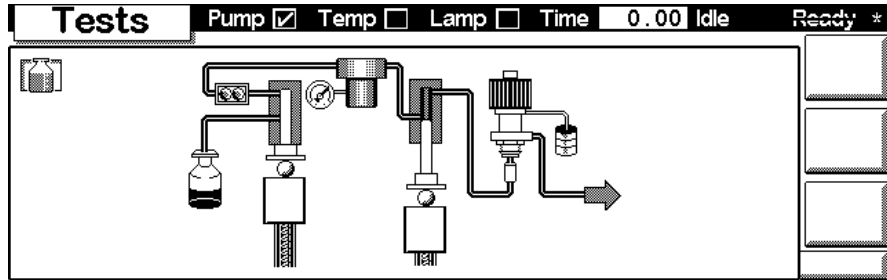

Diagnostics and Tests


Tests screen

Use the Esc key to receive **Views** on the F5 key. Choose **System** from the pull-down menu. Use the F3 key (**Tests**) to select the pump. Two tests are available to test the Agilent 1100 pumps.

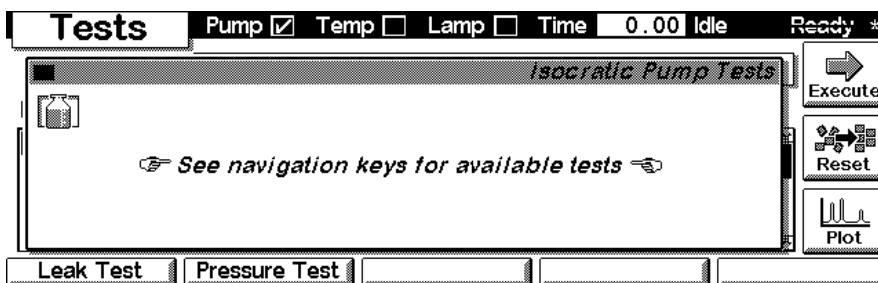


Leak Test

Press F1 (Leak Test) on the Test screen to perform a leak test. Several steps like purging the system, setting up Isopropanol as solvent and blocking the purge valve outlet with a blank nut have to be performed before operating the leak test. For details use the 'i'-key to achieve context sensitive help, follow the instructions on the screen and refer to "Leak Test" on page 81. For evaluating the pressure test refer to "Evaluating the Results" on page 79.

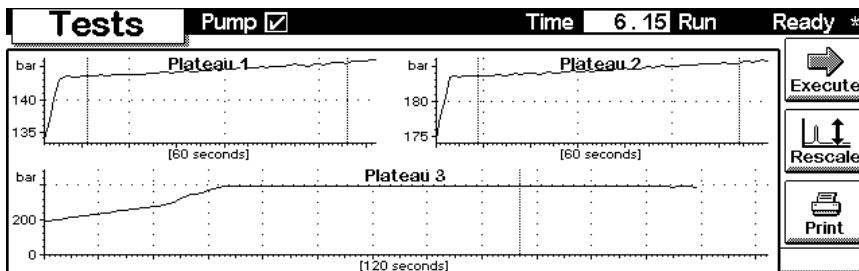

Pressure Test

Use the F2 key (**Pressure Test**) to perform a pressure test of the system. Several steps like purging the system, setting up Isopropanol as solvent and blocking the column outlet with a blank nut have to be performed before operating the pressure test. For details use the 'i'-key to achieve context sensitive help, follow the instructions on the screen and refer to [“Running the Pressure Test”](#) on page 77. For evaluating the pressure test refer to [“Evaluating the Results”](#) on page 79.

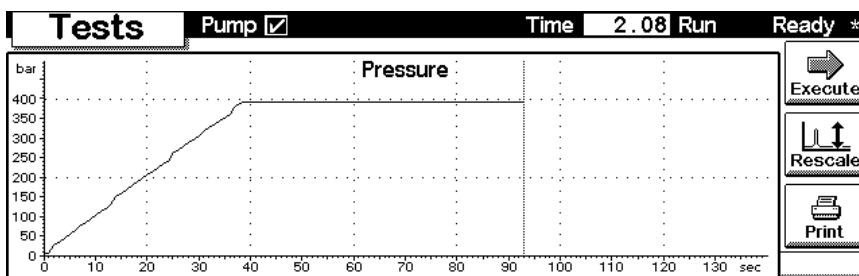



8 Specifications

Performance Specifications 246



Performance Specifications

Table 43 Performance Specification Agilent 1100 Series Isocratic Pump


Type	Specification
Hydraulic system	Dual piston in series pump with proprietary servo-controlled variable stroke drive, floating pistons and active inlet valve
Setable flow range	0.001 – 10 ml/min, in 0.001 ml/min increments
Flow range	0.2 – 10.0 ml/min
Flow precision	< 0.3 % RSD (typically 0.15 %), based on retention time, at 1 ml/min
Pressure	Operating range 0 – 40 MPa (0 – 400 bar, 0 – 5880 psi) up to 5 ml/min Operating range 0 – 20 MPa (0 – 200 bar, 0 – 2950 psi) up to 10 ml/min
Pressure pulsation	< 2 %amplitude (typically < 1 %), at 1 ml/min isopropanol, at all pressures > 10 bar (147 psi)
Compressibility compensation	User-selectable, based on mobile phase compressibility
Recommended pH range	1.0 – 12.5, solvents with pH > 2.3 should not contain acids which attack stainless steel
Control and data evaluation	Agilent ChemStation for LC
Control and data evaluation	Agilent ChemStation for LC
Analog output	For pressure monitoring, 2 mV/bar, one output
Communications	Controller-area network (CAN), GPIB, RS-232C, APG Remote: ready, start, stop and shut-down signals, LAN optional
Safety and maintenance	Extensive diagnostics, error detection and display (through control module and Agilent ChemStation), leak detection, safe leak handling, leak output signal for shutdown of pumping system. Low voltages in major maintenance areas.

Table 43 Performance Specification Agilent 1100 Series Isocratic Pump (continued)

GLP features	Early maintenance feedback (EMF) for continuous tracking of instrument usage in terms of seal wear and volume of pumped mobile phase with user-settable limits and feedback messages. Electronic records of maintenance and errors.
Housing	All materials recyclable.

NOTE

For use with flow rates below 500 $\mu\text{l}/\text{min}$ a vacuum degasser is required.

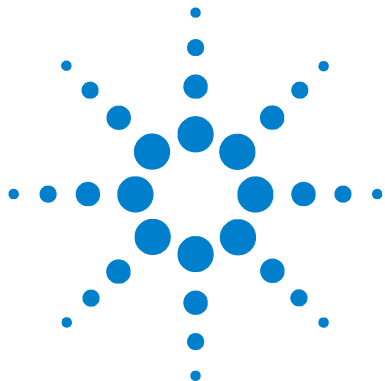

A Safety Information

General Safety Information	250
Lithium Batteries Information	253
Radio Interference	254
Sound Emission	255
Solvent Information	256
Agilent Technologies on Internet	257



General Safety Information

The following general safety precautions must be observed during all phases of operation, service, and repair of this instrument. Failure to comply with these precautions or with specific warnings elsewhere in this manual violates safety standards of design, manufacture, and intended use of the instrument. Agilent Technologies assumes no liability for the customer's failure to comply with these requirements.

General

This is a Safety Class I instrument (provided with terminal for protective earthing) and has been manufactured and tested according to international safety standards.

Operation

Before applying power, comply with the installation section. Additionally the following must be observed.

Do not remove instrument covers when operating. Before the instrument is switched on, all protective earth terminals, extension cords, auto-transformers, and devices connected to it must be connected to a protective earth via a ground socket. Any interruption of the protective earth grounding will cause a potential shock hazard that could result in serious personal injury. Whenever it is likely that the protection has been impaired, the instrument must be made inoperative and be secured against any intended operation.

Make sure that only fuses with the required rated current and of the specified type (normal blow, time delay, and so on) are used for replacement. The use of repaired fuses and the short-circuiting of fuseholders must be avoided.

Some adjustments described in the manual, are made with power supplied to the instrument, and protective covers removed. Energy available at many points may, if contacted, result in personal injury.

Any adjustment, maintenance, and repair of the opened instrument under voltage should be avoided as much as possible. When inevitable, this should be carried out by a skilled person who is aware of the hazard involved. Do not

attempt internal service or adjustment unless another person, capable of rendering first aid and resuscitation, is present. Do not replace components with power cable connected.

Do not operate the instrument in the presence of flammable gases or fumes. Operation of any electrical instrument in such an environment constitutes a definite safety hazard.

Do not install substitute parts or make any unauthorized modification to the instrument.




Capacitors inside the instrument may still be charged, even though the instrument has been disconnected from its source of supply. Dangerous voltages, capable of causing serious personal injury, are present in this instrument. Use extreme caution when handling, testing and adjusting.

When working with solvents please observe appropriate safety procedures (e.g. goggles, safety gloves and protective clothing) as described in the material handling and safety data sheet by the solvent vendor, especially when toxic or hazardous solvents are used.

Safety Symbols

Table 44 shows safety symbols used on the instrument and in the manuals.

Table 44 Safety Symbols

Symbol	Description
	The apparatus is marked with this symbol when the user should refer to the instruction manual in order to protect the apparatus against damage.
	Indicates dangerous voltages.
	Indicates a protected ground terminal.

WARNING

A warning alerts you to situations that could cause physical injury or damage to the equipment. Do not proceed beyond a warning until you have fully understood and met the indicated conditions.

CAUTION

A caution alerts you to situations that could cause a possible loss of data. Do not proceed beyond a caution until you have fully understood and met the indicated conditions.

Lithium Batteries Information

WARNING

Danger of explosion if battery is incorrectly replaced. Replace only with the same or equivalent type recommended by the equipment manufacturer. Lithium batteries may not be disposed-off into the domestic waste.

Transportation of discharged Lithium batteries through carriers regulated by IATA/ICAO, ADR, RID, IMDG is not allowed. Discharged Lithium batteries shall be disposed off locally according to national waste disposal regulations for batteries.

WARNING

Lithiumbatteri - Eksplosionsfare ved fejlagtig handling. Udskiftning må kun ske med batteri af samme fabrikat og type. Lever det brugte batteri tilbage til leverandoren.

WARNING

Lithiumbatteri - Eksplosionsfare. Ved udskiftning benyttes kun batteri som anbefalt av apparatfabrikanten. Brukt batteri returneres apparatleverandoren.

NOTE

Bij dit apparaat zijn batterijen geleverd. Wanneer deze leeg zijn, moet u ze niet weggoien maar inleveren als KCA.



Radio Interference

Never use cables other than the ones supplied by Agilent Technologies to ensure proper functionality and compliance with safety or EMC regulations.

Test and Measurement

If test and measurement equipment is operated with equipment unshielded cables and/or used for measurements on open set-ups, the user has to assure that under operating conditions the radio interference limits are still met within the premises.

Sound Emission

Manufacturer's Declaration

This statement is provided to comply with the requirements of the German Sound Emission Directive of 18 January 1991.

This product has a sound pressure emission (at the operator position) < 70 dB.

- Sound Pressure $L_p < 70$ dB (A)
- At Operator Position
- Normal Operation
- According to ISO 7779:1988/EN 27779/1991 (Type Test)

Solvent Information

Observe the following recommendations on the use of solvents.


Flow Cell

Avoid the use of alkaline solutions (pH > 11) which can attack quartz and thus impair the optical properties of the flow cell.

Solvents

Always filter solvents, small particles can permanently block the capillaries. Avoid the use of the following steel-corrosive solvents:

- Solutions of alkali halides and their respective acids (for example, lithium iodide, potassium chloride, and so on).
- High concentrations of inorganic acids like nitric acid, sulfuric acid especially at higher temperatures (replace, if your chromatography method allows, by phosphoric acid or phosphate buffer which are less corrosive against stainless steel).
- Halogenated solvents or mixtures which form radicals and/or acids, for example:



This reaction, in which stainless steel probably acts as a catalyst, occurs quickly with dried chloroform if the drying process removes the stabilizing alcohol.

- Chromatographic grade ethers, which can contain peroxides (for example, THF, dioxane, di-isopropylether) such ethers should be filtered through dry aluminium oxide which adsorbs the peroxides.
- Solutions of organic acids (acetic acid, formic acid, and so on) in organic solvents. For example, a 1-% solution of acetic acid in methanol will attack steel.
- Solutions containing strong complexing agents (for example, EDTA, ethylene diamine tetra-acetic acid).
- Mixtures of carbon tetrachloride with 2-propanol or THF.

Agilent Technologies on Internet

For the latest information on products and services visit our worldwide web site on the Internet at:

<http://www.agilent.com/go/chem>

Select “Products” - “Chemical Analysis”

It will also provide the latest firmware of the Agilent 1100 series modules for download.

A Safety Information

Index

A

- accessory kit, 16
- active inlet valve, 94, 168
- active inlet valve drive, 202
- adapter, 94, 96, 156
- air flow, 132
- algae, 30
- algae growth, 32
- alternative seal material, 36
- ambient non-operating temperature, 14
- ambient operating temperature, 14
- analog output, 246
- APG remote connector, 20, 213
- ASIC - application-specific integrated circuit, 202
- assembling the main cover, 145
- AUTO mode, 195
- AUX output, 20

B

- ball-screw drive, 192
- battery, 203, 253
- baudrate setting, 218
- BCD board, 116, 208
- bench space, 13
- blank nut, 77
- blockage, 63
- board connectors, 122
- bottle, 15
- bottle head assembly, 15, 155
- buffer application, 30
- buffer solutions, 190

C

- cable
 - CAN, 15, 20
 - GPIB, 20
 - power, 15
 - remote, 15

- signal, 16
- CAN cable, 20
- CAN interface, 212
- capillary, pump to injection device, 16
- changing solvents, 25
- ChemStation, 20
- cleaning the pump, 91
- columns, 190
- compensation sensor open, 52
- compensation sensor short, 53
- compensation volume, 195
- compressibility compensation, 37, 194, 246
- condensation, 13
- connections, flow, 22
- continuous seal wash, 35, 190
- control module, 151, 153
 - EMF, 237
 - firmware update, 238
 - serial number change of MWD, 240
 - tests, 243
- counter, EMF, 199
- counter, seal wear, 199
- cover parts, 157

D

- damaged parts, 15
- damper, 129
- damping unit, 129
- data bit settings, 218
- default address settings, 217
- delay volume, 17, 194
- delivery checklist, 15
- description, leak test, 81
- description, pressure test, 76
- dimensions, 13
- dual-piston in-series design, 191

E

- early maintenance feedback (EMF), 198

- electrical connections
 - descriptions of, 196
- electronic fuses, 203
- electrostatic discharge (ESD), 90
- EMF
 - on control module, 237
- EMF counters, 199
- EMF limits, 200
- encoder missing, 64
- environment, 12, 13
- error
 - zero solvent counter, 57
- error condition, 43
- error message
 - wait timeout, 75
- error messages, 40, 44
 - compensation sensor open, 52
 - compensation sensor short, 53
 - encoder missing, 64
 - fan failed, 54
 - ignition without cover, 55
 - index adjustment, 71
 - index limit, 70
 - index missing, 72
 - initialization failed, 74
 - inlet valve fuse, 62
 - inlet-valve missing, 65
 - leak, 49
 - leak sensor open, 50
 - leak sensor short, 51
 - missing pressure reading, 61
 - motor drive power, 63
 - pressure above upper limit, 58
 - pressure below lower limit, 59
 - pump head missing, 69
 - restart without cover, 56
 - selection valve failed, 60
 - servo restart failed, 68
 - shut-down, 46
 - stroke length, 73
 - synchronization lost, 47
 - temperature limit exceeded, 67

Index

- temperature out of range, 66
- timeout, 45
- error
 - unknown error 2055, 57
- ESD (electrostatic discharge) strap, 91
- ESD wrist strap, 16
- exchanging
 - active inlet valve, 93, 94
 - damper, 129
 - fan, 132
 - interface board, 116
 - internal parts, 90, 117
 - leak sensor, 142
 - LPM board, 121
 - outlet ball valve, 93, 98
 - pistons, 93, 106
 - power supply, 137
 - pump drive, 134
 - pump seals, 93
 - purge valve, 93, 100
 - purge valve frit, 93, 100
 - status light pipe, 144
 - wash seals, 93, 108
- Exchanging the Active Inlet Valve Cartridge, 96
- F**
 - fan, 132
 - fan drive, 202
 - fan failed, 54
 - fan out, 213
 - features
 - GLP, 247
 - instrument layout, 198
 - safety and maintenance, 246
 - firmware
 - description, 206
 - main system, 206
 - resident system, 206
 - firmware update with control module, 238
 - flow connections, 22
 - flow precision, 246
 - flow range, 246
 - foam, 146
 - foam parts, 159
 - frequency range, 13
 - front of pump, 19
 - fuse, electronic, 203
- G**
 - GPIB
 - Default Addresses, 217
 - GPIB cable, 20
 - GPIB interface, 212
 - gradient valve drive, 202
- H**
 - hex key set, 16
 - hexagonal key, 4 mm, 102, 103, 106, 108, 112, 115
 - highest injection precision, 34
 - highest precision, 30
 - hints for successful use, 30
 - humidity, 14
 - hydraulic path, 156
 - hydraulic system, 246
- I**
 - index adjustment, 71
 - index limit, 70
 - index missing, 72
 - initialization, 193
 - initialization failed, 74
 - inlet-valve fuse, 62
 - inlet-valve missing, 65
 - installation, pump module, 19
 - instrument status
 - indicator, 43
 - lamp, 43
 - interface
 - CAN, 212
 - GPIB, 212
 - remote, 213
 - RS-232C, 214
 - interface board, 116
 - interface boards, optional, 208
 - interfaces, 203
 - internal parts, 117
- L**
 - laboratory bench, 13
 - lamp
 - instrument status, 43
 - lamp, power supply, 42
 - lamp, status, 41
 - LAN cables, 187
 - LAN interface board, 209
 - leak, 49
 - leak converter, 202
 - leak parts, 161
 - leak sensor, 142
 - leak sensor open, 50
 - leak sensor short, 51
 - leak test, 40, 81
 - light pipes, 160
 - line frequency, 13
 - line voltage, 13
 - liter counters, counter, liter, 199
 - lithium battery, 253
 - logbook, 44
 - low-pressure pump main board (LPM), 202
 - LPM board, 121
- M**
 - main assemblies, 150
 - main assemblies, overview, 92
 - main board, 121
 - main power supply, 221
 - main power supply specification, 222
 - maintenance procedures, 199
 - materials in contact with mobile phase, 194
 - message
 - ignition without cover, 55
 - missing parts, 15
 - missing pressure reading, 61
 - motor drive, 202
 - motor-drive power, 63
- N**
 - non-operating altitude, 14
 - non-operating temperature, 14
 - not-ready condition, 43
- O**
 - onboard battery, 203
 - operating altitude, 14
 - operating temperature, 14
 - optimum performance, 17

optional interface board, 208
 outlet ball valve, 98, 166
 outlet capillary, 156
 overview, pump, 191

P

parity settings, 219
 parts
 active inlet valve, 168
 bottle head assembly, 155
 control module, 151, 153
 cover, 157
 damaged, 15
 foam, 159
 hydraulic path, 156
 leak handling, 161
 light pipes, 160
 main assemblies, 150
 missing, 15
 outlet ball valve, 166
 pump head, 162
 pump head with seal wash, 164
 pump housing and main assemblies, 150, 151
 sheet metal kit, 158
 solvent cabinet, 154
 parts identification
 cables - LAN cables, 187
 performance specification, 246
 pH range, 246
 physical specifications, 13
 piston, 30, 106, 192
 piston chamber, 191
 plateaus, leak test, 86
 power consideration, 12
 power consumption, 14
 power cords, 12
 power light pipe, 160
 power supply, 137
 power supply indicator, 42
 power supply lamp, 42
 power switch, 19
 power-input socket, 12
 prerin condition, 43
 pressure above upper limit, 58
 pressure below lower limit, 59
 pressure converter, 202
 pressure pulsation, 37, 195, 246

pressure range, 36
 pressure sensor readings, 20
 pressure test, 40, 76
 pressure, operating range, 246
 priming
 with a pump, 25, 26, 34
 with a syringe, 25, 34
 PTFE frit, 16, 100
 pump drive, 134
 pump head assembly, 162
 pump head missing, 69
 pump head with seal wash, 164
 pump piston, 30
 pump seals, 30
 purge valve, 30, 100
 purging the pump, 25

R

reassembling the pump head, 115
 recommended pH range, 246
 remote
 signal distribution, 213
 remote interface, 213
 removing
 pump head assembly, 102
 the foam, 118
 the top cover, 118
 repair procedures, 93
 repairs, 90
 using the ESD strap, 91
 replacing the foam, 146
 replacing the top cover, 146
 reproducibility, 30
 restart without cover, 56
 results, pressure test, 79
 RS-232
 cable kit to PC, 186
 RS-232C communication settings, 218
 RS-232C connection table, 214
 RS-232C interface, 214
 run mode, 43
 running the leak test, 83
 running the pressure test, 77

S

safety
 standards, 14

safety light switch, 120, 146
 sapphire piston, 192
 screwdriver pozidriv #1, 118, 129, 146
 screwdriver, pozidriv #1, 132, 137, 142, 144
 seal
 wear-in, 105
 seal insert tool, 16
 seal wash, 35, 191
 seal wash, when to use, 35
 seal wear counters, 199
 seal, alternative material, 36
 seals, 30, 103, 106, 108, 112, 115
 security lever, 19, 90
 selection valve failed, 60
 serial number
 entered on control module, 240
 serial number change with control module, 240
 servo restart failed, 68
 setable flow range, 246
 setting
 baudrate, 218
 data bit, 218
 forced cold-start, 219
 parity, 219
 RS 232C communication, 218
 stay resident, 220
 setting the address, 217
 sheet metal kit, 158
 shipping containers, 15
 shut-down, 46
 simple repair procedures, 93
 simple repairs, 90
 site requirements, 12
 snap fasteners, 22
 solvent bottle, 15
 solvent cabinet, 15, 30, 154
 solvent filters
 checking, 32
 cleaning, 33
 prevent blocking, 32
 solvent information, 31
 solvent inlet filters, 30
 sonic bath, 98
 specification
 main power supply, 222
 performance, 246
 physical, 13

Index

- spectrum
 - range, [230](#)
- stack configuration, [17](#)
- stack configuration, front view, [17](#)
- stack configuration, rear view, [18](#)
- status indicator, [41](#)
- status indicators, [40](#)
- status lamp, [41](#)
- status light pipe, [144](#), [160](#)
- stay resident settings, [220](#)
- stroke length, [73](#)
- stroke volume, [192](#), [195](#)
- synchronization lost, [47](#)
- syringe adapter, [25](#)
- wideranging capability, [12](#)
- wrench 1/4 inch, [77](#), [83](#), [98](#), [100](#), [102](#),
[103](#), [106](#), [108](#), [112](#), [115](#), [129](#)
- wrench 14 mm, [94](#), [96](#), [98](#), [100](#)
- wrench, 1/4 - 5/16 inch, [16](#)
- wrench, 1/4 inch, [142](#)
- wrench, 14 mm, [16](#), [121](#), [142](#)
- wrench, 5 mm, [142](#)
- wrench, 7 mm, [129](#), [132](#), [137](#), [142](#), [144](#),
[146](#)

Z

- zero solvent counter, [57](#)

T

- temperature limit exceeded, [67](#)
- temperature out of range, [66](#)
- temperature sensor, [49](#)
- tests on control module, [243](#)
- timeout, [45](#)
- top cover, [145](#), [146](#)

U

- unknown error 2055, [57](#)
- unpacking the pump, [15](#)

V

- vacuum degasser, [30](#), [190](#), [247](#)
- vacuum degasser, operational hints, [34](#)
- vacuum degasser, when to use, [34](#)
- valve frit, [100](#)
- variable reluctance motor, [192](#)
- variable stroke volume, [195](#)
- velocity regulator, [16](#), [35](#)
- voltage range, [13](#)
- voltage selector, [12](#)

W

- wait timeout, [75](#)
- wall socket, [12](#)
- waste tube, [16](#)
- wear-in
 - procedure, [105](#)
- weight, [13](#)



In This Book

This manual contains technical reference information about the Agilent 1100 Series isocratic pump. The manual describes the following:

- installation,
- optimizing performance,
- diagnostics and troubleshooting,
- repairing,
- parts and materials,
- introduction, theory of operation,
- screens of local control module and
- specifications.

